

Maintenance Manual

Field Master™ MS2070A/MS2080A

Handheld Spectrum Analyzer

The Anritsu logo is located in the bottom right corner of the page. It consists of the word "Anritsu" in a bold, blue, sans-serif font. The letter "A" is stylized with a diagonal slash through it.

NOTICE

Anritsu Company has prepared this manual for use by Anritsu Company personnel and customers as a guide for the proper installation, operation and maintenance of Anritsu Company equipment and computer programs. The drawings, specifications, and information contained herein are the property of Anritsu Company, and any unauthorized use or disclosure of these drawings, specifications, and information is prohibited; they shall not be reproduced, copied, or used in whole or in part as the basis for manufacture or sale of the equipment or software programs without the prior written consent of Anritsu Company.

UPDATES

The latest service and sales contact information, and updated documents can be downloaded from the Anritsu Website at: <http://www.anritsu.com>

Notes On Export Management

This product and its manuals may require an Export License or approval by the government of the product country of origin for re-export from your country.

Before you export this product or any of its manuals, please contact Anritsu Company to confirm whether or not these items are export-controlled.

When disposing of export-controlled items, the products and manuals need to be broken or shredded to such a degree that they cannot be unlawfully used for military purposes.

Table of Contents

Chapter 1— General Information

1-1	Introduction	1-1
	Additional Documentation	1-1
1-2	Contacting Anritsu	1-2
1-3	Required Test Equipment and Tools	1-2
1-4	Replaceable Parts	1-3

Chapter 2—Spectrum Analyzer Verification

2-1	Introduction	2-1
	PASS/FAIL Determination for Instrument Key Parameter Performance Tests	2-2
2-2	Frequency Accuracy	2-3
	Without GPS Connection	2-3
	With GPS Connection (Option 31)	2-4
2-3	Amplitude Accuracy	2-5
	Amplitude Accuracy – Preamplifier Off	2-5
	Amplitude Accuracy – Preamplifier On	2-7
2-4	Single Side Band (SSB) Phase Noise	2-8
2-5	Second Harmonic Distortion	2-10
2-6	Displayed Average Noise Level (DANL)	2-11
	DANL – Preamplifier Off	2-11
	DANL – Preamplifier On	2-13
2-7	Residual Spurs	2-15
	Residual Spurs – Preamplifier On	2-15
	Residual Spurs – Preamplifier Off	2-17
2-8	Input Related Spurious	2-19

Chapter 3—Battery Information

3-1	General Information	3-1
3-2	Battery Pack Removal and Replacement	3-2

Chapter 4—Assembly Replacement

4-1	Introduction	4-1
4-2	Replaceable Parts List	4-1
4-3	Battery Pack Removal and Replacement	4-2
4-4	Bumpers Removal	4-3
4-5	Rear Case Removal	4-4
4-6	Touchscreen/LCD Removal	4-5
4-7	SPA PCB Assembly Removal	4-9
4-8	Main PCB Removal	4-11

Table of Contents (Continued)

4-9	Fan Assembly Removal	4-12
4-10	RF Input Adapter Removal	4-13
4-11	Reassembling the Unit	4-14

Chapter 5—Troubleshooting

5-1	Introduction	5-1
5-2	Level Accuracy Problems	5-1

Appendix A—Test Records

A-1	Introduction	A-1
A-2	Test Records for Spectrum Analyzer Verification	A-1

Chapter 1 — General Information

1-1 Introduction

This manual provides the recommended test equipment and tools, replaceable parts list, verification procedures, part replacement procedures, maintenance instructions, and test record templates for the MS2070A/80A Anritsu Field Master.

Familiarity with the basic operation is assumed (for example, how to change measurement modes, preset the instrument, and set up measurements).

This manual includes:

- General information including:
 - Required Test Equipment and Tools listed in [Table 1-2 on page 1-2](#) and [Table 1-3 on page 1-3](#).
 - Replaceable Parts listed in [Table 1-4 on page 1-3](#).
- Performance verification procedures included in [Chapter 2, “Spectrum Analyzer Verification”](#).
- Assembly replacement and troubleshooting procedures:
 - [Chapter 4, “Assembly Replacement”](#)
 - [Chapter 5, “Troubleshooting”](#)
- Blank test records are included in [Appendix A](#).
 - Copy the blank test records from [Appendix A](#) and use them to record measured values. Anritsu recommends making a copy of the blank test records to document measurements each time a performance verification is performed. Continuing to document this process each time provides a detailed history of the instrument performance.

Note

The MS2070A/80A performance verification procedures are provided in [Chapter 2](#) and [Chapter 4](#). Test records templates are provided in [Appendix A](#). Copy the test records templates and use them to record the measured values obtained when verifying the performance of the MS2070A/80A. The measurement values taken and documented provide a record of the performance of your instrument. Anritsu recommends that you make a copy of the test records to document the measurements each time a Performance Verification is performed. Continuing to document this process each time it is performed provides a detailed history of instrument performance.

Additional Documentation

Table 1-1. Related Manuals

Document Part Number	Description
10100-00069	Important Product Information, Compliance, and Safety Notices
11410-02892	Field Master™ MS2070A Technical Data Sheet
11410-01001	Field Master MS2080A Technical Data Sheet
10580-00483	Field Master MS2070A/80A User Guide
10580-00484	Field Master MS2080A Programming Manual
10580-00495	Field Master MS2070A Programming Manual

Updates, if any, can be downloaded from the Library tab on the Anritsu product page:

<https://www.anritsu.com/en-us/test-measurement/products/ms2080a>

<https://www.anritsu.com/en-us/test-measurement/products/ms2070a>

1-2 Contacting Anritsu

To contact Anritsu, visit the following URL and select the services in your region:

<http://www.anritsu.com/contact-us>

1-3 Required Test Equipment and Tools

Table 1-2 provides a list of the test equipment used for the performance verification tests of the instrument. The test equipment is critical in making accurate measurements. In some cases, you may substitute certain test equipment having the same critical specifications as the test equipment indicated in the test equipment list.

Table 1-3 provides the list of tools that may be required to remove the screws and nuts of the instrument.

Table 1-2. Required Test Equipment

Instrument / Component	Critical Specification	Recommended Manufacturer / Model
Synthesizer	9 kHz to 20 GHz	Anritsu MG36221A
Power Meter	18 GHz	Rohde and Schwarz, NRP18T
Termination	50 Ω , N Type	Anritsu 28N50-2
Low Pass Filter	50 MHz	Mini-Circuits, NLP-50
10 MHz Reference	10 MHz	Datum / 9390-6000
Power Splitter	N Type	Weinschel 1870A
Adapter	N Type	Anritsu 34NN50A
Adapter	SMA(m) to BNC(f)	Anritsu 2000-2054-R
Adapter	Ruggedized K(m) to N(f)	Anritsu 34RKNF50
Attenuator, Qty 2	N Type, 10 dB	Weinschel 44-10
Attenuator, Qty 1	N Type 20 dB	Weinschel 44-20
Coaxial Cable	BNC(m) to BNC(m)	Pomona
RF Coaxial Cable, Qty 1	N Type	Anritsu 15NN50-1.5C

Table 1-3. Required Tools

Tools	Specification
Wrench	5/16"
Torx Screwdriver	T10
Torx Screwdriver	T 20
Phillips Screwdriver	#1
Phillips Screwdriver	#2
Nut Driver	5.5 mm
Hex Socket Driver	6 mm (1/4")

1-4 Replaceable Parts

The MS2070A/80A replacement parts and their description are listed below in [Table 1-4](#).

Table 1-4. List of Replaceable Parts (1 of 2)

Part Number	Description
3-ND87053-RFB	MS2080A Main
3-ND88096	MS2080A SPA PCB, Rev 2
3-ND87446-RFB	MS2070A Main
3-ND88143	MS2070A SPA PCB, Rev 2
3-ND87258-RFB	SPA PCB, Rev 1
3-ND87055	LCD Top Case Assembly
3-ND87259	Battery Door
3-85716-1-0	Bottom Case
3-ND87261	Connector Panel, Rev 1
3-ND88098	Connector Panel, Rev 2
3-ND87260	Fan Assembly
3-ND87341	Tilt Bail Assembly
3-806-195	Battery Cable
3-85721	Battery Shroud
3-ND87340	Wi-Fi Antenna
633-79	Li-Ion Battery
40-204-R	AC/DC Adapter
3-513-100	RF Input Port
2000-2002-R	External Power Pack
3-74842-3	Keypad Cable
3-806-415	Shielded LCD Cable
3-85093	Stand-Offs
3-85719	Left Bumper
3-85720	Right Bumper
3-85718-4	MS2080A Model Label 4 GHz
3-85718-6	MS2080A Model Label 6 GHz

Table 1-4. List of Replaceable Parts (2 of 2)

Part Number	Description
3-87338-3	MS2070A Model Label 3 GHz

Chapter 2 — Spectrum Analyzer Verification

2-1 Introduction

This chapter provides the verification procedures for the MS2070A/80A Field Master. Verification tests that are associated with other instrument options are described in [Chapter 4, “Assembly Replacement”](#). Record the measurement results in the test record templates provided in [Appendix A, “Test Records”](#).

This chapter includes the following performance verification procedures:

- [Section 2-2 “Frequency Accuracy” on page 2-3](#)
- [Section 2-3 “Amplitude Accuracy” on page 2-5](#)
- [Section 2-4 “Single Side Band \(SSB\) Phase Noise” on page 2-8](#)
- [Section 2-5 “Second Harmonic Distortion” on page 2-10](#)
- [Section 2-6 “Displayed Average Noise Level \(DANL\)” on page 2-11](#)
- [Section 2-7 “Residual Spurs” on page 2-15](#)
- [Section 2-8 “Input Related Spurious” on page 2-19](#)

PASS/FAIL Determination for Instrument Key Parameter Performance Tests

Figure 2-1 shows the rule that is used to determine the pass/fail status of test results that are associated with warranted specifications.

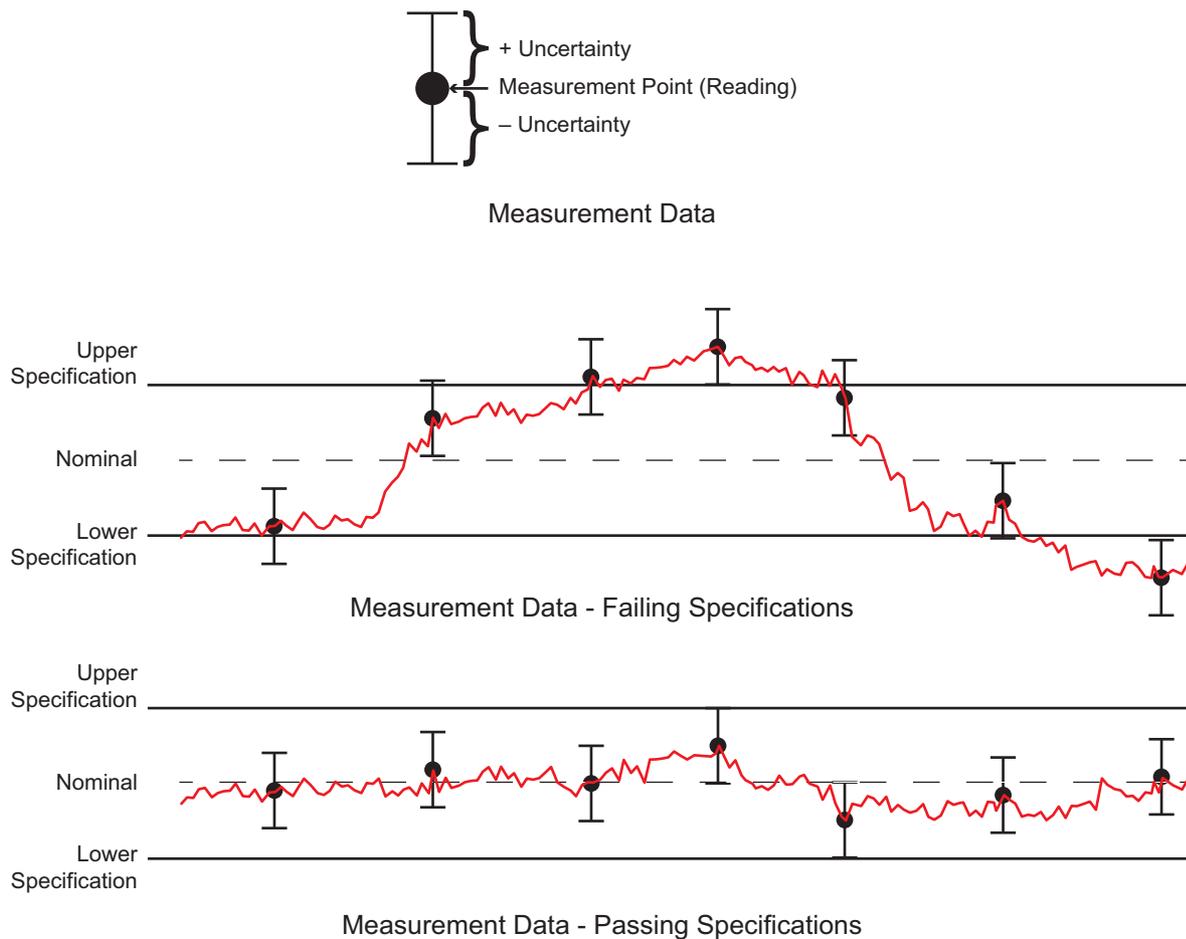


Figure 2-1. Pass/Fail Determination

The measurement uncertainty listed in each test record includes the best estimate of the errors contributed by the measurement, test equipment, standards, and other correction factors (for example, calibration factors and mismatch error) based on the suggested equipment, the equipment setup, and the prescribed test procedure. Most of the uncertainties are type-B per ISO/IEC Guide 98-3, Guide to the Expression of Uncertainty in Measurement (GUM).

2-2 Frequency Accuracy

Use the following procedures to verify the frequency accuracy of the MS2070A/80A., without and with GPS connection. Record the results in the test records provided in [Appendix A](#)

There are two procedures involved in verifying the frequency accuracy:

- “Without GPS Connection”
- “With GPS Connection (Option 31)”

Note Before continuing, allow a 30 minute warm-up for the internal circuitry to stabilize.

Without GPS Connection

Use the following procedures to verify the frequency accuracy of the MS2070A/80A without GPS connection.

Equipment Required

- Anritsu MG36221A Synthesizer
- Anritsu 15NN50-1.5C RF Coaxial Cable
- Anritsu 34RKNF50 Ruggedized K(m) to N(f) Adapter
- 10 MHz Frequency Reference
- BNC(m) to BNC(m) Coaxial Cable
- SMA(m) to BNC(f) Adapter

Procedure

1. Connect the external 10 MHz frequency reference to the MG36221A.

Note Do not connect the 10 MHz Reference to the MS2070A/80A.

2. Connect the MG36221A RF Out to the MS2070A/80A RF In.
3. Set the MG36221A RF output as follows:
 - Power Level: –30 dBm
 - CW Frequency: 1 GHz
4. Set the MS2070A/80A to spectrum analyzer mode and preset the instrument (PRESET > Preset Mode).
5. Set the MS2070A/80A parameters as follows:
 - Center Frequency: 1 GHz
 - Span: 10 kHz
 - Reference Level: –10 dBm
 - RBW: 30 Hz
 - VBW: 3 Hz
6. Enable Marker 1 and perform a Peak Search. Record the marker frequency in [Table A-1, “MS2070A/80A Spectrum Analyzer Frequency Accuracy \(without GPS\)”](#) on page A-1. Calculate the error by subtracting 1 GHz from the measured value and record the error in [Table A-1](#) on page A-1.

With GPS Connection (Option 31)

Use this procedure to verify the frequency accuracy of the MS2070A/80A. Record the results in the test records provided in [Appendix A](#).

Equipment Required

- Anritsu MG36221A Synthesizer
- 10 MHz Frequency Reference
- Anritsu 34RKNF50 Adapter
- Anritsu 15NN50-1.5C RF Coaxial Cable
- SMA(m) to BNC(f) Adapter
- BNC(m) to BNC(m) Coaxial Cable
- GPS antenna

Procedure

1. Connect the external 10 MHz Reference to the MG36221A.

Note Do not connect the 10 MHz Reference to the MS2070A/80A.

2. Connect the MG36221A RF Out to the MS2070A/80A RF In.
3. Set the MG36221A RF output as follows:
 - Power Level: -30 dBm
 - CW Frequency: 1 GHz
4. Connect the GPS antenna to the MS2070A/80A, and confirm GPS coordinates are shown where the message “No GPS Fix” was shown prior to connecting the antenna.
5. Set the MS2070A/80A parameters as follows:
 - Center Frequency: 2 GHz for MS2070A
 - Center Frequency: 3 GHz for MS2080A
 - Span: 10 kHz
 - Reference Level: -10 dBm
 - RBW: 30 kHz
 - VBW: 3 Hz
 - Sweep Once
6. Enable Marker 1 and perform a Peak Search. Record the marker frequency in [Table A-2, “MS2070A Option 31, GPS Frequency Accuracy” on page A-1](#). Calculate the error by subtracting 2 GHz from the measured value and record the error in [Table A-3 on page A-1](#).
7. Enable Marker 1 and perform a Peak Search. Record the marker frequency in [Table A-3, “MS2080A Option 31, GPS Frequency Accuracy” on page A-1](#). Calculate the error by subtracting 1 GHz from the measured value and record the error in [Table A-3 on page A-1](#).

2-3 Amplitude Accuracy

Use the following procedures to verify the amplitude accuracy of the MS2070A/80A and record the results in the test records provided in [Appendix A](#).

There are two procedures involved in verifying the amplitude accuracy:

- “[Amplitude Accuracy – Preamplifier Off](#)”
- “[Amplitude Accuracy – Preamplifier On](#)”

Note Before continuing, allow a 30 minute warm-up for the internal circuitry to stabilize.

Amplitude Accuracy – Preamplifier Off

Use the following procedure to verify the amplitude accuracy of the MS2070A/80A with preamplifier off.

Equipment Required

- Anritsu MG36221A Synthesizer
- Weinschel 1870A Power Splitter
- Weinschel 44-10 Attenuator
- Rohde and Schwarz NRP18T Power Sensor
- Anritsu 15NN50-1.5C RF Coaxial Cable
- Anritsu 34NN50A Adapter
- Anritsu 34RKNF50 Adapter
- SMA(m) to BNC(f) Adapter
- BNC(m) to BNC(m) Coaxial Cable
- 10 MHz Frequency Reference

Procedure

1. Connect the external 10 MHz Reference to both the MG36221A and MS2070A/80A.
2. Connect the MG36221A RF Out to the input of the splitter.
3. Connect the NRP18T directly to one output of the splitter.
4. Connect the 10 dB attenuator to the other output of the splitter.
5. Connect the RF input of the MS2070A/80A to the 10 dB attenuator.
6. Set the MS2070A/80A to spectrum analyzer mode and preset the instrument (PRESET > Preset Mode).
7. Set the MS2070A/80A parameters as follows:
 - Span: 10 kHz
 - Reference Level: 10 dBm
 - Attenuation Level: 30 dB
 - Preamplifier: Off
 - RBW: 1 kHz
 - VBW: 10 Hz
 - Detector Type: Peak
8. Using the Rohde and Schwarz Power Viewer software, set the signal frequency to 50 MHz.
9. On the MG36221A, press RF OFF.

10. Zero the NRP18T sensor.
11. On the MG36221A, press RF ON.
12. On the MG36221A, set the frequency to 50 MHz.
13. Adjust the NRP18T power level to +10.0 dBm. (The power level reading of MG36221A should be approximately +16 dBm.)
14. Set the MS2070A/80A center frequency to 50 MHz.
15. Perform a marker peak search and record the amplitude in [Table A-4, “MS2070A/80A Power Level Accuracy at 50 MHz \(Preamplifier Off\)”](#) on page A-2
16. Adjust the Reference Level and Attenuation Level on the MS2070A/80A for the other values in [Table A-4, “MS2070A/80A Power Level Accuracy at 50 MHz \(Preamplifier Off\)”](#) on page A-2
17. Adjust the Power Level on the MG36221A for the other power levels in [Table A-4, “MS2070A/80A Power Level Accuracy at 50 MHz \(Preamplifier Off\)”](#) on page A-2, and record results for each measurement.
18. Repeat this procedure for the other frequencies using the tables listed below:
 - [Table A-4, “MS2070A/80A Power Level Accuracy at 50 MHz \(Preamplifier Off\)”](#) for all frequency options

Amplitude Accuracy – Preamplifier On

Use the following procedure to verify the amplitude accuracy of the MS2070A/80A with the preamplifier on. Record the results in the test records provided in [Appendix A](#).

Note Before continuing, allow a 30 minute warm-up for the internal circuitry to stabilize.

Equipment Required

- Anritsu MG36221A Synthesizer
- SMA(m) to BNC(f) Adapter
- Weinschel 1870A Power Splitter
- Weinschel 44-10 Attenuator, Qty 2
- Weinschel 44-20 Attenuator
- Rohde and Schwarz NRP18T Power Sensor
- Anritsu 15NN50-1.5C RF Coaxial Cable
- Anritsu 34NN50A Adapter, N(m) to N(m)
- Ruggedized 34RKNF50 Adapter, K(m) to N(f)
- 10 MHz Frequency Reference
- BNC(m) to BNC(m) Coaxial Cable

Procedure

1. Connect the external 10 MHz Reference to both the MG36221A and MS2070A/80A.
2. Connect the MG36221A RF Out to the input of the splitter.
3. Connect the NRP18T directly to one output of the splitter.
4. Connect 40 dB of attenuation to the other output of the splitter.
5. Connect the RF input of the MS2070A/80A to the 40 dB attenuation.
6. Set the MS2070A/80A to spectrum analyzer mode and preset the instrument (PRESET > Preset Mode).
7. Set the MS2070A/80A parameters as follows:
 - Span: 10 kHz
 - Reference Level: -40 dBm
 - Attenuation Level: 0 dB
 - Preamplifier: On
 - RBW: 1 kHz
 - VBW: 10 Hz
 - Detector Type: Peak
8. Using the Rohde and Schwarz Power Viewer software, set the signal frequency to 100 kHz. Ensure the MG36221A is not outputting any power, and zero the NRP18T sensor.
9. On the MG36221A, set the frequency to 100 kHz and adjust the power level so the NRP18T measures -10 dBm. (The MG36221A should be approximately -4 dBm.)
10. On the MS2070A/80A set the center frequency to 100 kHz and perform a peak search. Record the result in [Table A-5, “MS2070A/80A Power Level Accuracy \(Preamplifier On\)”](#) on page A-2.
11. Repeat [Step 8](#) through [Step 10](#) for the remaining frequencies that apply to the unit being tested, in [Table A-5, “MS2070A/80A Power Level Accuracy \(Preamplifier On\)”](#) on page A-2.

2-4 Single Side Band (SSB) Phase Noise

Use the following procedure to verify the single side-band (SSB) phase noise of the MS2070A/80A. Record the results in the test records provided in [Appendix A](#).

Note Before continuing, allow a 30 minute warm-up for the internal circuitry to stabilize.

Equipment Required

- Anritsu MG36221A
- Ruggedized 34RKNF50 Adapter, K(m) to N(f)
- SMA(m) to BNC(f) Adapter
- Anritsu 15NN50-1.5C Coaxial Cable, N(m) to N(m)
- 10 MHz Frequency Reference
- BNC(m) to BNC(m) coaxial cable

Procedure

1. Connect the external 10 MHz Reference to both the MG36221A and MS2070A/80A.
2. Connect the MG36221A RF Out to the MS2070A/80A RF In.
3. Set the MG36221A to output frequency to 1.0 GHz.
4. Set the MG36221A to output power to -2 dBm.
5. Set the MS2070A/80A to spectrum analyzer mode and preset the instrument (PRESET > Preset Mode).
6. Set the MS2070A/80A parameters as follows:
 - Reference Level: 0 dBm
 - Input Attenuation: 15 dB
 - Preamplifier: Off
 - RBW: 1 kHz
 - VBW: 3 Hz
 - Detector Type: Peak
 - Averages: 3
 - Sweep Points: 601
7. 10 kHz and 100 kHz Offset Settings:
 - Center Frequency: 1000.05 MHz
 - Span: 110 kHz
8. In the Sweep menu, turn off Continuous Sweep, and choose Sweep to three and allow it to finish.
9. In the Marker menu, use the Peak Search menu to set Marker 1 to the peak at 1 GHz. Exit the Peak Search menu and set the Marker Mode to Delta. Enter a frequency value of 10 kHz, so a marker is on the peak at 1 GHz and the delta marker is 10 kHz away. Record the difference in level between the peak at 1 GHz and the noise level 10 kHz away at 1000.010 MHz in [Table A-6, “MS2070A/80A Spectral Purity - SSB Phase Noise Offset from 1 GHz” on page A-3](#). Then subtract another 30 dB and record this as the 10 kHz Offset Measured Value reading in [Table A-6 on page A-3](#).

For example: -80 dBc measured $- 30$ dB = -110 dBc/Hz
10. Change the Delta Frequency from 10 kHz to 100 kHz and record the difference in level between the peak at 1 GHz and the noise level 100 kHz away at 1000.100 MHz in [Table A-6, “MS2070A/80A Spectral Purity - SSB Phase Noise Offset from 1 GHz” on page A-3](#). Then subtract another 30 dB and record this as the 100 kHz Offset Measured Value reading in [Table A-6, “MS2070A/80A Spectral Purity - SSB Phase Noise Offset from 1 GHz” on page A-3](#).

For example: $-80 \text{ dBc measured} - 30 \text{ dB} = -110 \text{ dBc/Hz}$

11. Change the Center Frequency to 1000.545 MHz and the Span to 1.1 MHz. Run the sweep of three averages and allow it to finish. Using Delta Markers, measure the difference in level between the peak at 1 GHz and the noise level 1 MHz away at 1001.0 MHz in [Table A-6, “MS2070A/80A Spectral Purity - SSB Phase Noise Offset from 1 GHz” on page A-3](#). Then subtract another 30 dB and record this as the 1 MHz Offset Measured Value reading in [Table A-6 on page A-3](#).

For example: $-85 \text{ dBc measured} - 30 \text{ dB} = -115 \text{ dBc/Hz}$

12. Change the Center Frequency to 1005.495 MHz and the Span to 11 MHz. Run the sweep of 3 averages and allow it to finish. Using Delta Markers, measure the difference in levels between the peak at 1 GHz and the noise level 10 MHz away at 1010 MHz in [Table A-6, “MS2070A/80A Spectral Purity - SSB Phase Noise Offset from 1 GHz” on page A-3](#). Then subtract another 30 dB and record this as the 10 MHz Offset Measured Value reading in [Table A-6 on page A-3](#).

For example: $-100 \text{ dBc measured} - 30 \text{ dB} = -130 \text{ dBc/Hz}$

2-5 Second Harmonic Distortion

Use the following procedure to verify the second harmonic distortion of the MS2070A/80A. Record the results in the test records provided in [Appendix A](#).

Note Before continuing, allow a 30 minute warm-up for the internal circuitry to stabilize.

Equipment Required

- Anritsu MG36221A Synthesizer
- Min-Circuits NLP-50 Low Pass Filter
- Anritsu 15NN50-1.5C RF Cable
- 10 MHz Frequency Reference
- BNC(m) to BNC(m) Coaxial Cable
- Ruggedized 34RKNF50 Adapter, K(m) to N(f)
- SMA(m) to BNC(f) Adapter

Procedure

1. Connect the 10 MHz reference to the MG36221A and MS2070A/80A.
2. Connect the output of the MG36221A to the input of the low pass filter and the output of the low pass filter to the RF In of the MS2070A/80A.
3. Set the MS2070A/80A to spectrum analyzer mode and preset the instrument (PRESET > Preset Mode).
4. Set the MS2070A/80A parameters as follows:
 - Center frequency: 50.1 MHz
 - Span: 100 kHz
 - Reference Level: -20 dBm
 - Attenuation Level: 0 dB
 - Preamplifier: Off
 - RBW: 1 kHz
 - VBW: 10 Hz
5. Set the MG36221A frequency to 50.1 MHz and adjust the level so the MS2070A/80A shows -30 dBm at 50.1 MHz. Record this value in [Table A-7, “MS2070A/80A Second Harmonic Distortion” on page A-3](#)
6. Set the MS2070A/80A Center Frequency to 100.2 MHz, perform a peak search, and record this value in [Table A-7 on page A-3](#).
7. Subtract 50.1 MHz value from the 100.2 MHz value and record this as the Second Harmonic Distortion in [Table A-7 on page A-3](#).

For example, if the 50.1 MHz value is -30 dBm and the 100.2 MHz value is -90 dBm, then:

$$-90 \text{ dBm} - (-30 \text{ dBm}) = -60 \text{ dBc}$$

2-6 Displayed Average Noise Level (DANL)

Use the following procedures to verify the Displayed Average Noise Level (DANL) of the MS2070A/80A. Record the results in the test records provided in [Appendix A](#).

There are two procedures involved in verifying the DANL of MS2070A/80A:

- “DANL – Preamplifier Off”
- “DANL – Preamplifier On”

DANL – Preamplifier Off

Use the following procedure to verify the Displayed Average Noise Level (DANL) of the MS2070A/80A with preamplifier off.

Note Before continuing, allow a 30 minute warm-up for the internal circuitry to stabilize.

Equipment Required

- Anritsu 28N50-2 Termination

MS2070A Procedure

1. Attach the Termination to the RF input of the MS2070A/80A.
2. Set the MS2070A to spectrum analyzer mode and preset the instrument (PRESET > Preset Mode).
3. Set the MS2070A parameters as follows:
 - Start Frequency: 10 MHz
 - Stop Frequency: 2 GHz
 - Reference Level: -20 dBm
 - Input Attenuation: 0 dB
 - Preamplifier: Off
 - RBW: 1 MHz
 - VBW: 1 kHz
 - VBW Type: Logarithmic
 - Detector Type: RMS/Avg
 - Sweep Points: 551
 - Continuous: Toggle Off
 - Press Sweep Once.
4. Using the Marker menu, choose Peak Search, subtract 60 dB from the measurement, and record the power level in [Table A-8](#), “MS2070A Displayed Average Noise Level (Preamplifier Off)” on page A-3
5. Change the start frequency to 2 GHz and stop frequency to 3 GHz and repeat [Step 3](#) and [Step 4](#) to record the power level in [Table A-9](#), “MS2080A Displayed Average Noise Level (Preamplifier Off)” on page A-3.

MS2080A Procedure

1. Attach the Termination to the RF input of the MS2080A.
2. Set the MS2080A to spectrum analyzer mode and preset the instrument (PRESET > Preset Mode).
3. Set the MS2080A parameters as follows:
 - Start Frequency: 10 MHz
 - Stop Frequency: 2 GHz
 - Reference Level: -20 dBm
 - Input Attenuation: 0 dB
 - Preamplifier: Off
 - RBW: 1 MHz
 - VBW: 1 kHz
 - VBW Type: Logarithmic
 - Detector Type: RMS/Avg
 - Sweep Points: 551
 - Continuous: Toggle Off
 - Press Sweep Once.
4. Using the Marker menu, choose Peak Search, subtract 60 dB from the measurement, and record the power level in [Table A-10, “MS2070A Displayed Average Noise Level \(Preamplifier On\)”](#) on page A-4.
5. Change the start frequency to 3 GHz and stop frequency to 4 GHz and repeat [Step 3](#) and [Step 4](#) to record the power level in [Table A-11, “MS2080A Displayed Average Noise Level \(Preamplifier On\)”](#) on page A-4.

DANL – Preamplifier On

Use the following procedure to verify the Displayed Average Noise Level (DANL) of the MS2070A/80A with the Preamplifier On. Record the results in the test records provided in [Appendix A](#).

Note Before continuing, allow a 30 minute warm-up for the internal circuitry to stabilize.

Equipment Required

- Anritsu 28N50-2 Termination

MS2070A Procedure

1. Attach the Termination to the RF input of the MS2070A.
2. Set the MS2070A to spectrum analyzer mode and preset the instrument (PRESET > Preset Mode).
3. Set the MS2070A parameters as follows:
 - Start Frequency: 10 MHz
 - Stop Frequency: 2 GHz
 - Reference Level: -50 dBm
 - Attenuation Level: 0 dB
 - Preamplifier: On
 - RBW: 1 MHz
 - VBW: 1 kHz
 - VBW Type: Logarithmic
 - Detector Type: RMS/Avg
 - Sweep Points: 551
 - Continuous: Toggle Off
 - Press Sweep Once.
4. Using the Marker menu, choose Peak Search, subtract 60 dB from the measurement, and record the power level in [Table A-10](#), “MS2070A Displayed Average Noise Level (Preamplifier On)” on [page A-4](#).
5. Change the start frequency to 2 GHz and stop frequency to 3 GHz and repeat [Step 3](#) and [Step 4](#) to record the power level in [Table A-10](#), “MS2070A Displayed Average Noise Level (Preamplifier On)” on [page A-4](#).

MS2080A Procedure

1. Attach the Termination to the RF input of the MS2080A.
2. Set the MS2080A to spectrum analyzer mode and preset the instrument (PRESET > Preset Mode).
3. Set the MS2080A parameters as follows:
 - Start Frequency: 10 MHz
 - Stop Frequency: 2 GHz
 - Reference Level: -50 dBm
 - Attenuation Level: 0 dB
 - Preamplifier: On
 - RBW: 1 MHz
 - VBW: 1 kHz
 - VBW Type: Logarithmic
 - Detector Type: RMS/Avg
 - Sweep Points: 551
 - Continuous: Toggle Off
 - Press Sweep Once.
4. Using the Marker menu, choose Peak Search, subtract 60 dB from the measurement, and record the power level in [Table A-11, “MS2080A Displayed Average Noise Level \(Preamplifier On\)”](#) on page A-4.
5. Change the start frequency to 2 GHz and stop frequency to 4 GHz and repeat [Step 3](#) and [Step 4](#) to record the power level in [Table A-11, “MS2080A Displayed Average Noise Level \(Preamplifier On\)”](#) on page A-4.

2-7 Residual Spurs

Use the following procedures to verify the Residual Spurs of the MS2070A/80A with the preamplifier off and preamplifier on. Residual spurs are tested in multiple bands, record the results in the test records provided in [Appendix A](#).

There are two procedures involved in verifying the Residual Spurs:

- “Residual Spurs – Preamplifier On”
- “Residual Spurs – Preamplifier Off”

Note Before continuing, allow a 30 minute warm-up for the internal circuitry to stabilize.

Residual Spurs – Preamplifier On

Use the following procedure to verify the Residual Spurs of the MS2070A/80A with the Preamplifier On. Record the results in the test records provided in [Appendix A](#).

Note Before continuing, allow a 30 minute warm-up for the internal circuitry to stabilize.

Equipment Required

- Anritsu 28N50-2 Termination

MS2070A Procedure

1. Attach the Termination to the RF input of the MS2070A.
2. Set the MS2070A to spectrum analyzer mode and preset the instrument (PRESET > Preset Mode).
3. Set the MS2070A parameters as follows:
 - Start Frequency: >10 MHz
 - Stop Frequency: 500 MHz
 - Reference Level: -50 dBm
 - Attenuation Level: 0 dB
 - Preamplifier: On
 - RBW: 300 Hz
 - VBW: 100 Hz
 - Sweep Points: 601
 - Continuous: Toggle off
 - Press Sweep Once
4. Using the Marker menu, choose Peak Search and record the power level in [Table A-12, “MS2070A Residual Spurs \(Preamplifier On\)”](#) on page A-4.

MS2080A Procedure

1. Attach the Termination to the RF input of the MS2080A.
2. Set the MS2080A to spectrum analyzer mode and preset the instrument (PRESET > Preset Mode).
3. Set the MS2080A parameters as follows:
 - Start Frequency: >10 MHz
 - Stop Frequency: 500 MHz
 - Reference Level: -50 dBm
 - Attenuation Level: 0 dB
 - Preamplifier: On
 - RBW: 300 Hz
 - VBW: 100 Hz
 - Sweep Points: 601
 - Continuous: Toggle off
 - Press Sweep Once.
4. Using the Marker menu, choose Peak Search and record the power level in [Table A-13, “MS2080A Residual Spurs \(Preamplifier On\)”](#) on page A-5.
5. Refer to [Table A-13a, “MS2080A Residual Spurs \(Preamplifier On, for Rev1 Option 704 models only\)”](#) on page A-5, for Rev1 Option 704 models.

Residual Spurs – Preamplifier Off

Use the following procedure to verify the Residual Spurs of the MS2070A/80A with the Preamplifier Off and Record the results in the test records provided in [Appendix A](#).

Equipment Required

- Anritsu 28N50-2 Termination

MS2070A Procedure

1. Attach the Termination to the RF input of the MS2070A.
2. Set the MS2070A to spectrum analyzer mode and preset the instrument (PRESET > Preset Mode).
3. Set the MS2070A parameters as follows:
 - Start Frequency: 10 MHz
 - Stop Frequency: 500 MHz
 - Reference Level: -50 dBm
 - Attenuation Level: 0 dB
 - Preamplifier: Off
 - RBW: 300 Hz
 - VBW: 100 Hz
 - Sweep Points: 601
 - Continuous: Toggle off
 - Press Sweep Once.
4. Using the Marker menu, choose Peak Search and record the power level in [Table A-14, “MS2070A Residual Spurs \(Preamplifier Off\)”](#) on page A-5.

MS2080A Procedure

1. Attach the Termination to the RF input of the MS2080A.
2. Set the MS2080A to spectrum analyzer mode and preset the instrument (PRESET > Preset Mode).
3. Set the MS2080A parameters as follows:
 - Start Frequency: 10 MHz
 - Stop Frequency: 500 MHz
 - Reference Level: -50 dBm
 - Attenuation Level: 0 dB
 - Preamplifier: Off
 - RBW: 300 Hz
 - VBW: 100 Hz
 - Sweep Points: 601
 - Continuous: Toggle off
 - Press Sweep Once.
4. Using the Marker menu, choose Peak Search and record the power level in [Table A-15, “MS2080A Residual Spurs \(Preamplifier Off\)”](#) on page A-6.
5. Change the Start Frequency to 3 GHz and Stop Frequency to 4 GHz.
6. Repeat [Step 3](#) and [Step 4](#) and record the power level in [Table A-15, “MS2080A Residual Spurs \(Preamplifier Off\)”](#) on page A-6.
7. Refer to [Table A-15a, “MS2080A Residual Spurs \(Preamplifier Off, for Rev1 Option 704 models only\)”](#) on page A-6 for Rev1 Option 704 models only.

2-8 Input Related Spurious

Use the following procedure to verify the Input Related Spurious of the MS2070A/80A. Record the results in the test records provided in [Appendix A](#).

Note Before continuing, allow a 30 minute warm-up for the internal circuitry to stabilize.

Equipment Required

- Anritsu MG36221A Synthesizer
- Anritsu 34RKNF50 Adapter
- Anritsu 15NNF50-1.5C RF Cable
- 10 MHz Frequency Reference
- BNC(m) to BNC(m) Coaxial Cable
- SMA(m) to BNC(f) Adapter

MS2070A Procedure

1. Connect the 10 MHz Reference to the MG36221A and MS2070A.
2. Connect the output of the MG36221A to the RF In of the MS2070A/80A.
3. Set the MS2070A/80A to spectrum analyzer mode and Preset the instrument (PRESET > Preset Mode).
4. Set the MS2070A parameters as follows:
 - Center Frequency: 2086 MHz
 - Span: 100 kHz
 - Reference Level: -30 dBm
 - Attenuation Level: 0 dB
 - Preamplifier: Off
 - RBW: 1 kHz
 - VBW: 10 Hz
5. Set the MG36221A frequency to 2086 MHz, and set power level so -30 dBm is read on the MS2070A at 2086 MHz. Record the measured input signal level in [Table A-16, “MS2070A Input Related Spurious” on page A-6](#).
6. Change the center frequency of the MS2070A to 400.5 MHz and record the highest spur level in [Table A-16, “MS2070A Input Related Spurious” on page A-6](#).

MS2080A Procedure

1. Connect the 10 MHz Reference to the MG36221A and MS2080A.
2. Connect the output of the MG36221A to the RF In of the MS2080A.
3. Set the MS2080A to spectrum analyzer mode and preset the instrument (PRESET > Preset Mode).
4. Set the MS2080A parameters as follows:
 - Center Frequency: 742 MHz
 - Span: 100 kHz
 - Reference Level: -30 dBm
 - Attenuation Level: 0 dB
 - Preamplifier: Off
 - RBW: 1 kHz
 - VBW: 10 Hz
5. Set the MG36221A frequency to 742 MHz, and set power level so -30 dBm is read on the MS2080A at 742 MHz. Record the highest spur level in [Table A-17, “MS2080A Input Related Spurs” on page A-7](#).
6. Change the center frequency of the MS2080A to 3500.5 MHz and record the highest spur level in [Table A-17, “MS2080A Input Related Spurs” on page A-7](#).

Chapter 3 — Battery Information

3-1 General Information

This chapter provides the care and handling information of the Anritsu 633-79 Lithium-Ion batteries.

- The battery supplied with the Field Master may need charging before use. Before using the instrument, make sure to charge the internal battery using the AC-DC Adapter.
- Use only Anritsu approved battery packs.
- Recharge the battery only in the instrument or in an Anritsu approved charger.
- When the instrument or the charger is not in use, disconnect it from the AC power source.
- Do not charge batteries for longer than 24 hours. Overcharging may shorten battery life.
- If left unused a fully charged battery will discharge itself over time.
- Temperature extremes affect the ability of the battery to charge. Allow the battery to cool down or warm up as necessary before use or charging.
- Discharge the battery from time to time to improve battery performance and battery life.
- The battery can be charged and discharged hundreds of times, but it will eventually wear out.
- The battery may need to be replaced when the operating time between charging becomes noticeably shorter than normal.
- Never use a damaged or worn out charger or battery.
- Storing the battery in extreme hot or cold places will reduce the capacity and lifetime of the battery.
- Never short-circuit the battery terminals.
- Do not drop, mutilate or attempt to disassemble the battery.
- Do not dispose of batteries in a fire!
- Batteries must be recycled or disposed of properly. Do not place batteries in household garbage.
- Always use the battery for its intended purpose only.

Warning



This equipment is supplied with a rechargeable battery that could potentially leak hazardous compounds into the environment. These hazardous compounds present a risk of injury or loss due to exposure. Anritsu Company recommends removing the battery for long-term storage of the instrument and storing the battery in a leak-proof, plastic container. Follow the environmental storage requirements specified in the product data sheet.

3-2 Battery Pack Removal and Replacement

This section provides instructions for the removal and replacement of the instrument battery pack.

1. Locate the battery access door on the left side of the unit.
2. Push in and slide the battery access door to remove the battery access door.
3. Pull straight out on the lanyard to remove the battery pack from the instrument.
4. After inserting the new battery pack, press the battery access door to secure it

Note When inserting the battery, the battery contacts should face up and slide in first. If the battery door does not close tightly, it means that the battery may have been inserted incorrectly.



Figure 3-1. Battery Access Door Location and Removal

- 5.

6. With the battery access door removed, grasp the battery lanyard and pull the battery straight out of the unit as illustrated in [Figure 3-2](#).



Figure 3-2. Removing the Battery

Chapter 4 — Assembly Replacement

4-1 Introduction

This chapter describes opening and closing the Field Master case along with basic parts replacement steps. The sections are as follows:

- “Battery Pack Removal and Replacement”
- “Bumpers Removal”
- “Rear Case Removal”
- “Touchscreen/LCD Removal”
- “SPA PCB Assembly Removal”
- “Main PCB Removal”
- “Fan Assembly Removal”
- “RF Input Adapter Removal”
- “Reassembling the Unit”

4-2 Replaceable Parts List

Refer to [Table 1-4, “List of Replaceable Parts” on page 1-3](#) for the list of replacement parts. Refer to the following sections for basic replacement instructions.

Caution

Electrostatic Discharge (ESD) can damage the highly sensitive circuits in the instrument. All work should be performed in a static-safe work area.

Only qualified personnel should open the case and replace internal assemblies. Assemblies shown in [Table 1-4](#) are typically the only items that may be replaced. The assemblies are highly fragile, items that must be soldered may not be replaced without specialized training.

The Field Master contains components that can easily be damaged by electrostatic discharge (ESD). An ESD safe work area and proper ESD handling procedures that conform to ANSI/ESD S20.20-1999 or ANSI/ESD S20.20-2007 is mandatory to avoid ESD damage when handling sub-assemblies or components found in the instrument.

Repair of damage that is found to be caused by electrostatic discharge is not covered under warranty.

Caution

Removing the RF shield from PC boards or adjustment of screws on or near the shields may detune sensitive RF circuits and will result in degraded performance.

Note

Many of the procedures in this section are generic and apply to many similar instruments. Photos and illustrations used are representative and may show instruments other than the Field Master.

4-3 Battery Pack Removal and Replacement

This section provides instructions for the removal and replacement of the instrument battery pack.

1. Locate the battery access door on the left side of the unit.
2. Remove the battery door tab by sliding it to the left. See [Figure 4-1](#).



Figure 4-1. Battery Access Door Removal

3. With the battery access door removed, grab the battery lanyard and pull the battery straight out of the unit as illustrated in [Figure 4-2](#).



Figure 4-2. Removing the Battery

4-4 Bumpers Removal

The procedure below provides instructions for removing the bumpers of the instrument:

1. Remove the left and right bumpers by pulling them outward from the bottom. See [Figure 4-3](#).



Figure 4-3. Pulling of Side Bumpers

2. Detach the bumpers completely by lifting them upwards to remove from the unit. See [Figure 4-4](#).



Figure 4-4. Side Bumpers Removal

4-5 Rear Case Removal

The procedure below provides instructions for removing the rear case of the instrument:

1. Remove the battery as shown in [Section 4-3 “Battery Pack Removal and Replacement”](#) on page 4-2.
2. Remove the side bumpers as shown in [Section 4-4 “Bumpers Removal”](#) on page 4-3.
3. Using a T10 Torx screwdriver, remove the nine screws from the back of the instrument as shown in [Figure 4-5](#).



Figure 4-5. Rear Case Removal

4. With all screws removed, place the instrument face down on a stable flat work surface.
5. Gently pull the rear case apart from the front case.

4-6 Touchscreen/LCD Removal

This procedure provides instructions to replace LCD touchscreen. With the rear case removed as shown in [Section 4-5 “Rear Case Removal”](#) on page 4-4, the internal assemblies can be removed and replaced as explained below:

1. Remove the battery access door and the battery as described in [Section 4-3 “Battery Pack Removal and Replacement”](#) on page 4-2.
2. Remove the rear case as described in [Section 4-5 “Rear Case Removal”](#) on page 4-4.
3. Remove the five Torx screws securing the Main PCB and SPA PCB assemblies using a T20 Torx driver. See [Figure 4-6](#).

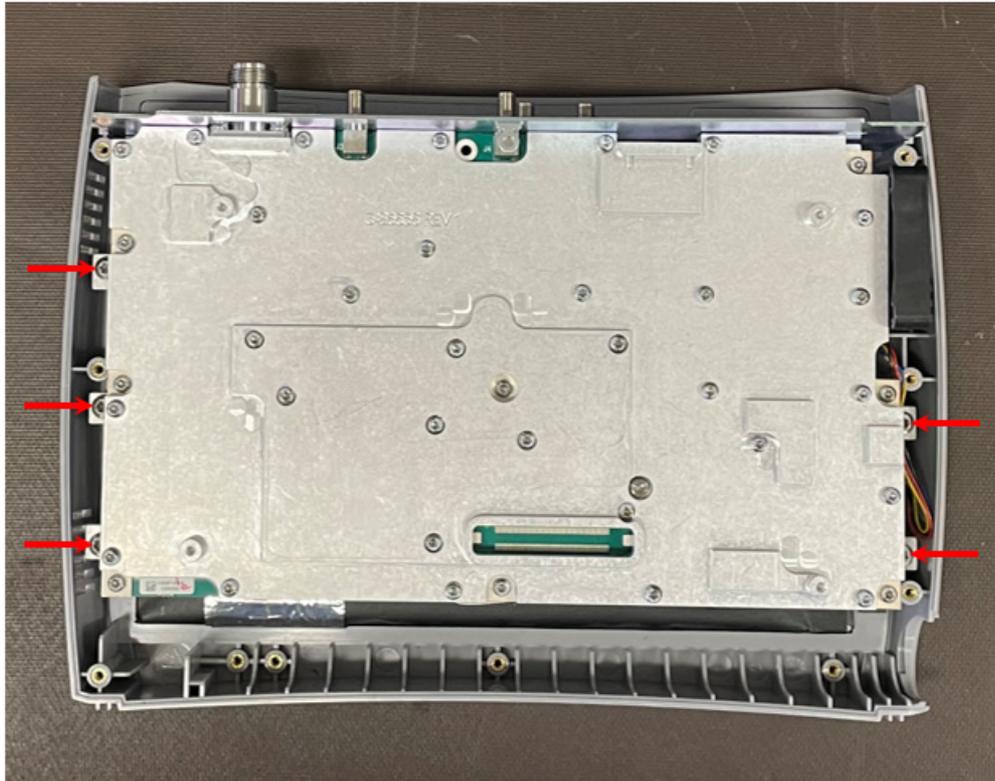


Figure 4-6. Main PCB/SPA PCB Removal

4. Remove the Torx screw on the top connector panel using a T10 screw driver. See [Figure 4-7](#).



Figure 4-7. Top Panel Removal

5. Remove the three Torx screws securing the battery shroud using a T10 Torx screw driver. See [Figure 4-8](#).

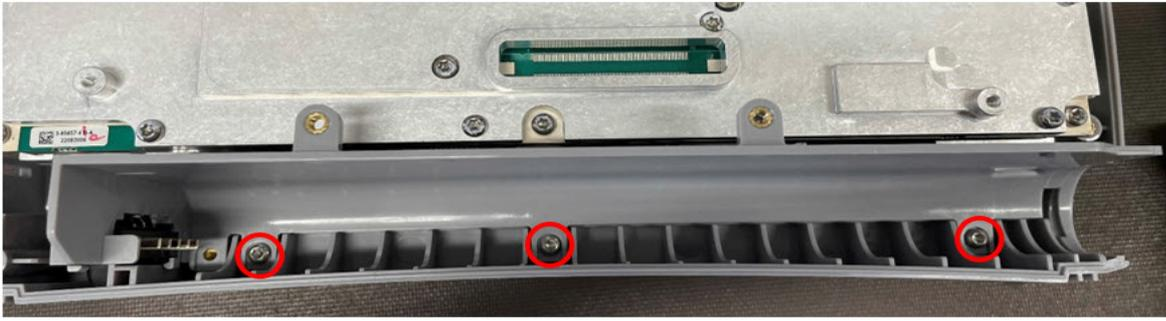


Figure 4-8. Battery Shroud Removal

6. Disconnect the battery cable and remove the battery shroud. See [Figure 4-9](#).

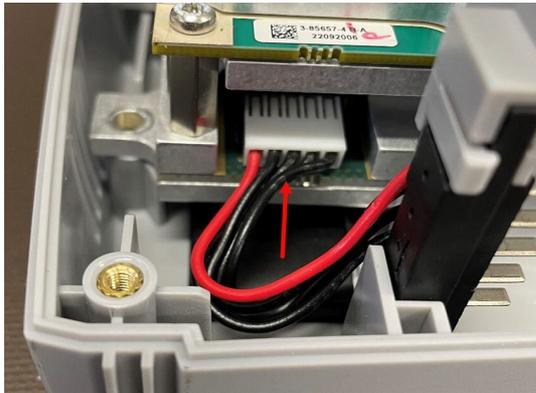


Figure 4-9. Battery Cable Removal

7. Carefully tilt the Main PCB/SPA PCB assembly to view the display cable. See [Figure 4-10](#).

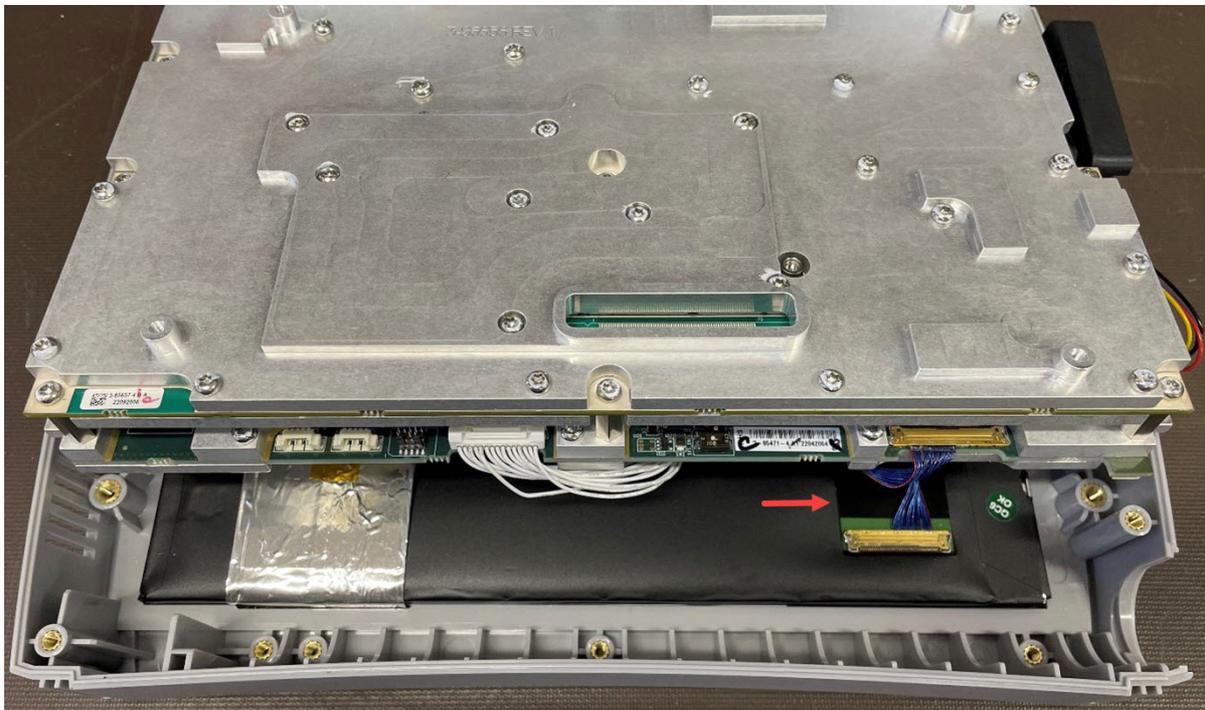


Figure 4-10. Display Cable

8. Release the locking connector by slowly lifting the metal flap upwards to disconnect the display cable. See [Figure 4-11](#).

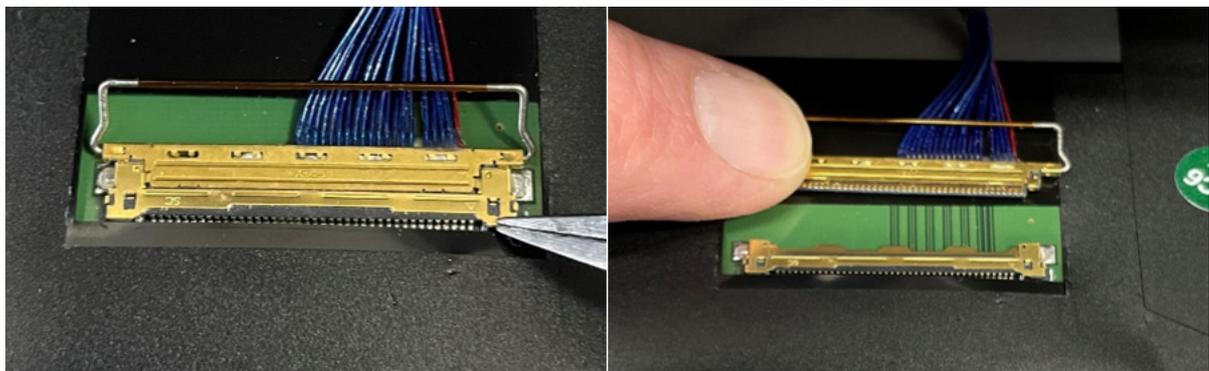


Figure 4-11. Display Cable Removal

9. Carefully tilt the Main PCB/SPA PCB assembly to remove the two Wi-Fi antennas. Release the Wi-Fi Antennas by carefully prying the end slots using a straight screw driver. See [Figure 4-12](#).



Figure 4-12. Releasing the Wi-Fi antennas

10. Carefully tilt the Main PCB/SPA PCB assembly to remove the keypad cable connector by slightly pressing it at the ends and disconnecting it from the LCD top case assembly. See [Figure 4-13](#).

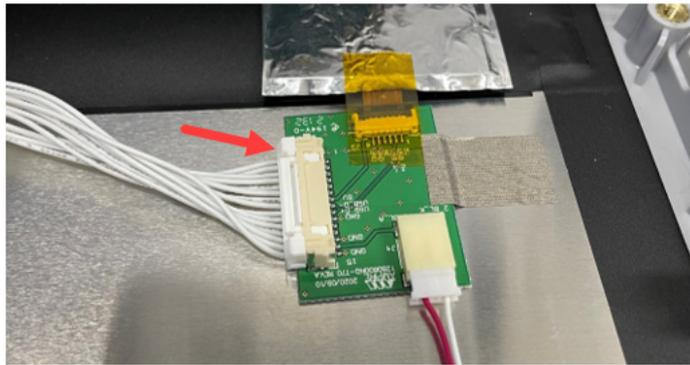


Figure 4-13. Disconnecting Keypad Cable Connector

11. The Touchscreen/LCD Display is permanently installed into the Top Case.

4-7 SPA PCB Assembly Removal

1. Remove the four nuts along with four lock washers from the SMA ports on the top connector panel using a 5/16" wrench. See [Figure 4-14](#).

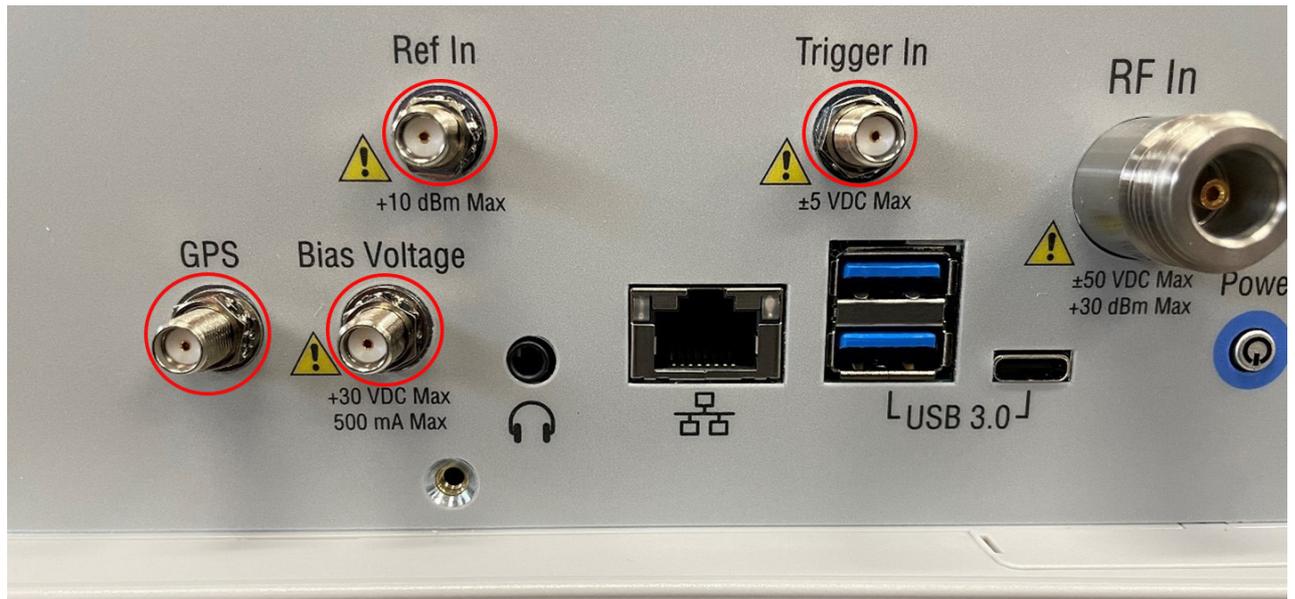


Figure 4-14. SPA PCB Removal

2. Remove the two Torx screws using T10 Torx driver from the brackets on the Main PCB. See [Figure 4-15](#).



Figure 4-15. SPA PCB Removal

3. Remove the eight Torx screws securing the SPA PCB Assembly to the Main PCB using a T10 Torx driver. See [Figure 4-16](#).

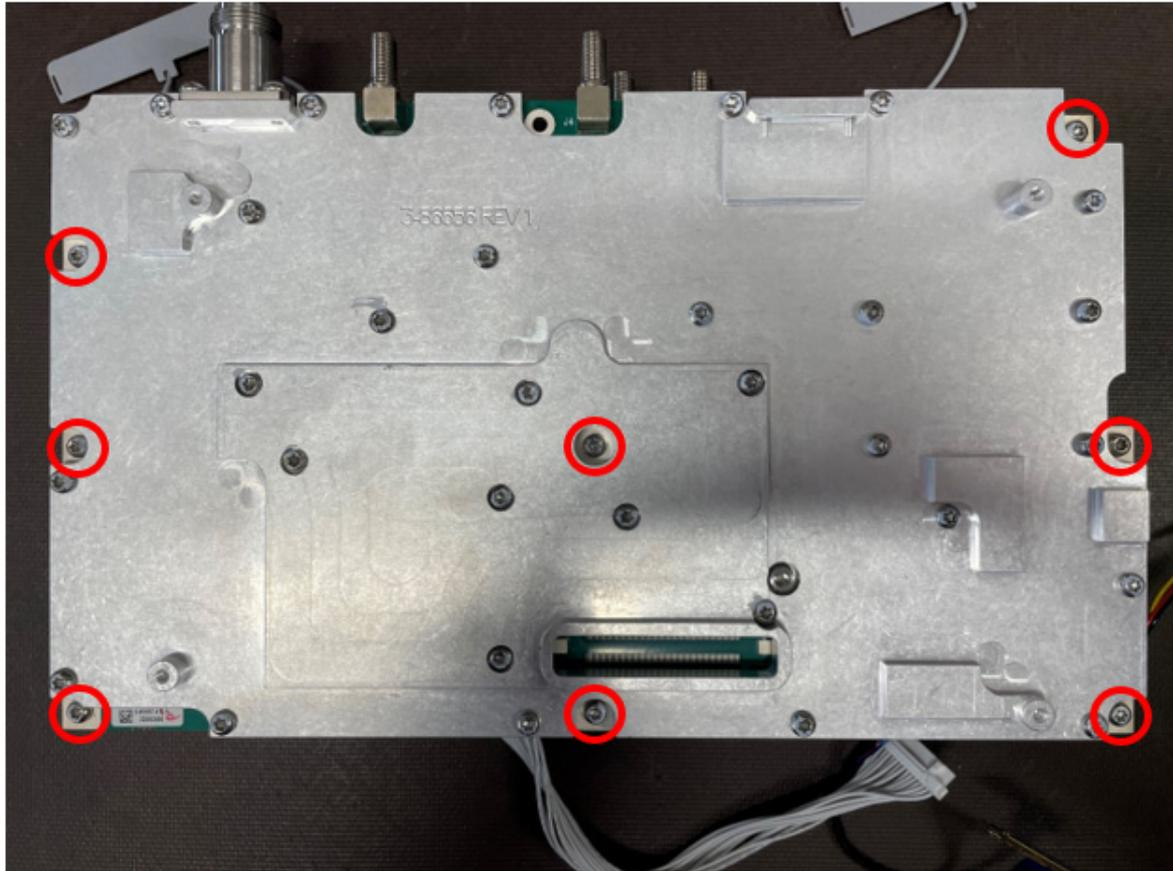


Figure 4-16. SPA PCB Removal: Torx Screws

4-8 Main PCB Removal

The semi-rigid cable connecting the RF input adapter and the step attenuator on the SPA PCB is normally a part of the SPA PCB Assembly, which may be replaced independently.

1. Carefully remove the two Wi-Fi cables, the keypad cable, and shielded LCD cable connected to the Main PCB.
2. Remove the eight stand-offs using 6 mm hex socket driver to remove the Main PCB. See [Figure 4-17](#).

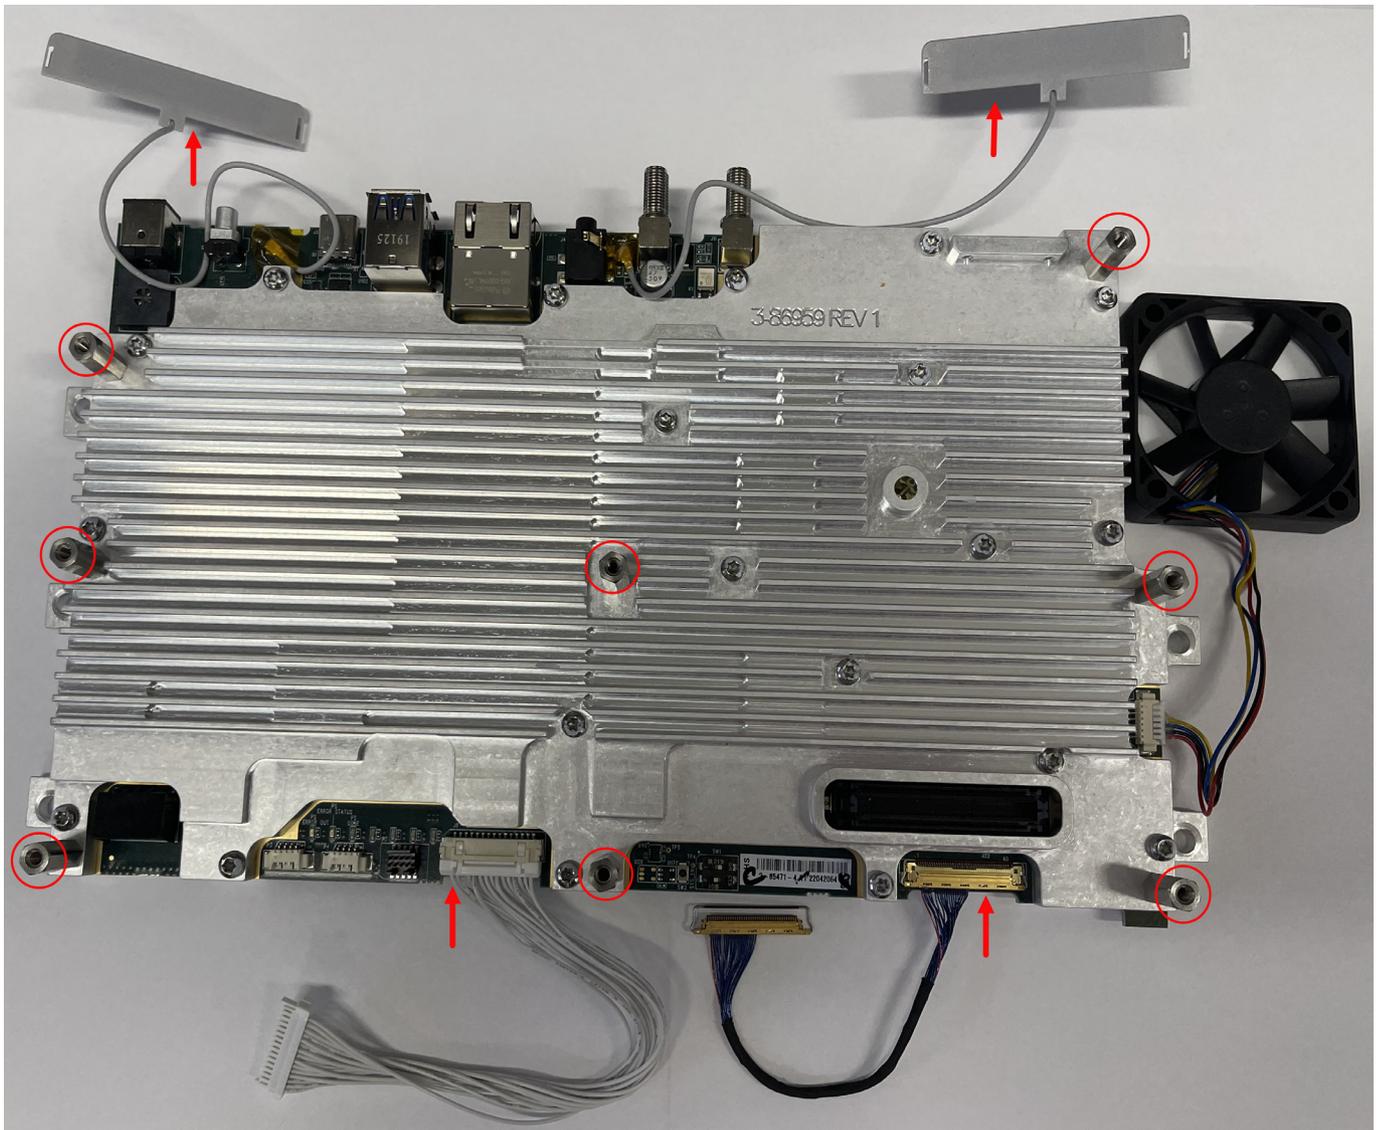


Figure 4-17. Main PCB Removal

4-9 Fan Assembly Removal

The fan assembly sits in a slot in the front case and is plugged into the Main PCB.

1. Carefully disconnect the harness and lift the fan assembly out of the case. See [Figure 4-18](#).

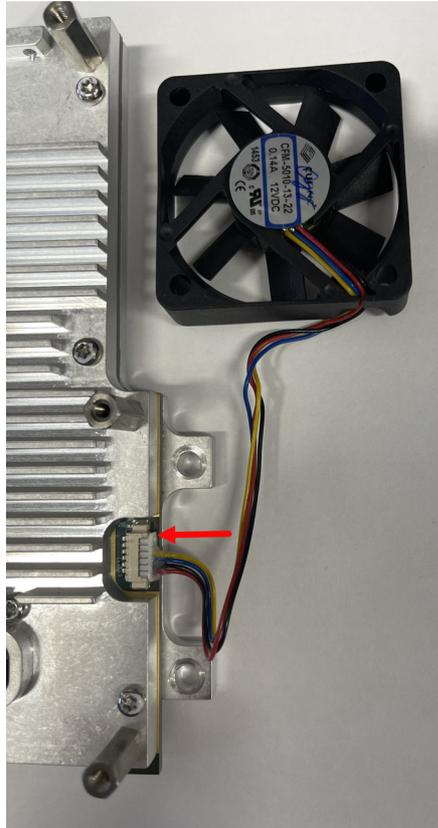


Figure 4-18. Fan Assembly Removal

4-10 RF Input Adapter Removal

The RF input adapter consists of four T10 Torx screws that are secured to the SPA PCB Assembly. Follow the steps below to remove the RF input adapter:

1. Using T10 Torx screw driver remove the four screws to carefully pull the RF input adapter straight off the SPA PCB assembly. See [Figure 4-19](#).

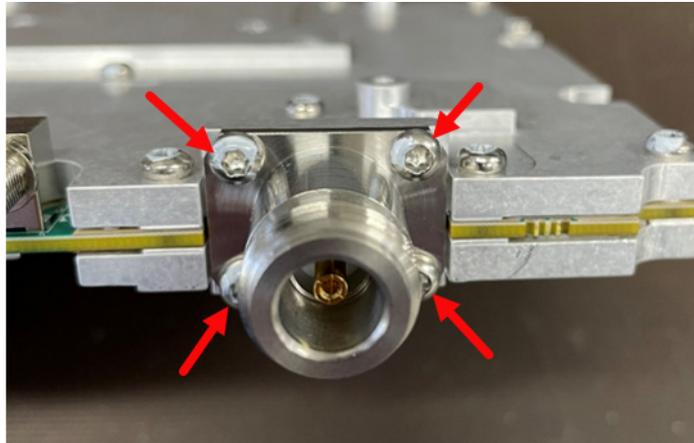


Figure 4-19. RF Input Adapter Removal

4-11 Reassembling the Unit

Reassembling the unit is simply a process done in the reverse order of the removal procedure. Use caution while reassembling all the parts together:

1. Ensure to carefully align the cables of the Wi-Fi antenna into the little grooves of the Main PCB to prevent the Wi-Fi antenna cables from being smashed or crimped. See [Figure 4-20](#).

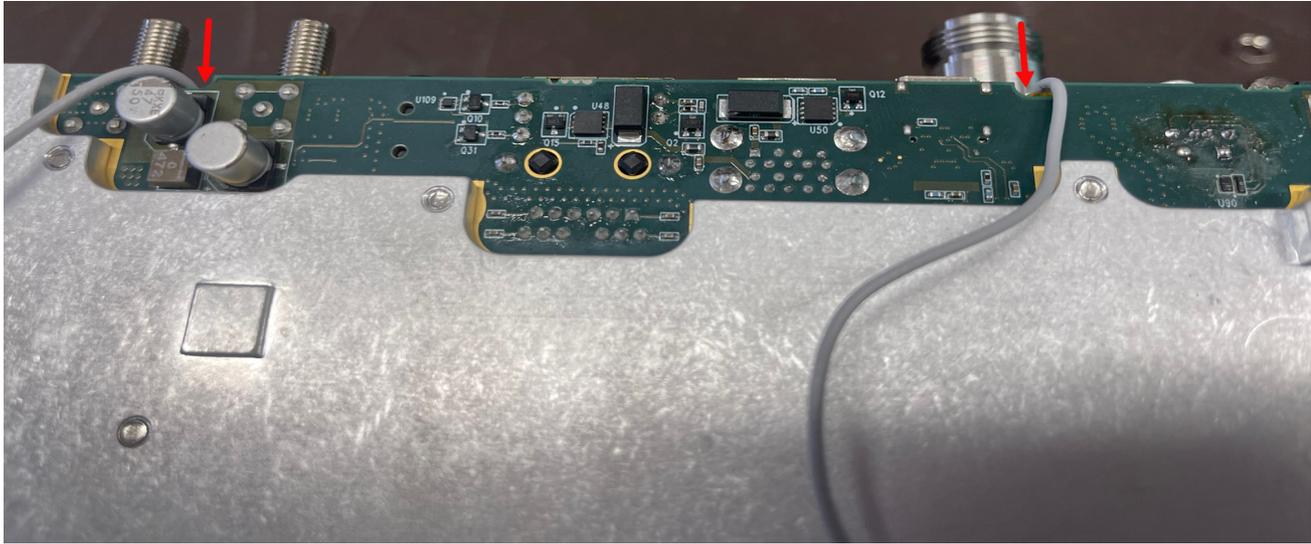


Figure 4-20. Reassembling the unit

2. Make sure that the label of the fan assembly faces outwards while fitting it into the LCD top case assembly. See [Figure 4-18](#).
3. Use caution as not to cripple the fan assembly harness in between while securing the Main PCB/SPA assembly onto the LCD Top case assembly. See [Figure 4-18](#).

Chapter 5 — Troubleshooting

5-1 Introduction

This chapter describes the primary troubleshooting operations that can be performed by all Anritsu service centers. Perform the troubleshooting suggestions in the order they are listed.

Only qualified Anritsu personnel should replace internal assemblies. Major subassemblies shown in [Table 1-4](#) are typically the items that may be replaced. Because they are highly fragile, items that must be soldered may not be replaced without special training. Removal of RF shields from PC boards or adjustment of screws on or near the shields will detune sensitive RF circuits and will result in degraded instrument performance.

5-2 Level Accuracy Problems

Measured signal is unexpectedly too high or too low:

1. Check the N connector for damage and cleanliness.
2. Check the connections between the N connector and Main PCB.
3. If the connections are good, replace the SPA PCB.

Appendix A — Test Records

A-1 Introduction

This appendix provides the test record templates to record the performance of the MS2070A/80A Field Master. Anritsu recommends that you make a copy of the following test record pages and document the measurements each time a performance verification is performed. Continuing to document this process each time it is performed provides a detailed history of instrument performance.

MS2070A/80A Firmware Rev: _____ Operator: _____ Date: _____

Serial Number: _____ Options: _____

A-2 Test Records for Spectrum Analyzer Verification

Table A-1. MS2070A/80A Spectrum Analyzer Frequency Accuracy (without GPS)

Frequency	Measured Value	Error	Measurement Uncertainty	Specification
1 GHz	GHz	Hz	250 Hz (0.25 ppm)	± 280 Hz (0.28 ppm)

Table A-2. MS2070A Option 31, GPS Frequency Accuracy

Frequency	Measured Value	Error	Measurement Uncertainty	Specification
2 GHz	GHz	Hz	30 Hz (15 ppb)	± 560 Hz (0.3 ppm)

Table A-3. MS2080A Option 31, GPS Frequency Accuracy

Frequency	Measured Value	Error	Measurement Uncertainty	Specification
3 GHz	GHz	Hz	45 Hz (15 ppb)	± 840 Hz (25 ppb)

MS2070A/80A Firmware Rev: _____ Operator: _____ Date: _____
 Serial Number: _____ Options: _____

Table A-4. MS2070A/80A Power Level Accuracy at 50 MHz (Preamplifier Off)

Frequency	Input Attenuation	Reference Level	NRP18T Power Level	MS2070A/80A Expected Power Level	MS2070A/80A Measured Power Level	Measurement Uncertainty	Specification
50 MHz	30 dB	10 dBm	+10 dBm	0 dBm	dBm	0.30 dB	0 dBm \pm 1.0 dB
50 MHz	30 dB	10 dBm	+6 dBm	-4 dBm	dBm	0.30 dB	-4 dBm \pm 1.0 dB
50 MHz	30 dB	10 dBm	+2 dBm	-8 dBm	dBm	0.30 dB	-8 dBm \pm 1.0 dB
50 MHz	20 dB	0 dBm	+0 dBm	-10 dBm	dBm	0.30 dB	-10 dBm \pm 1.0 dB
50 MHz	20 dB	0 dBm	-4 dBm	-14 dBm	dBm	0.30 dB	-14 dBm \pm 1.0 dB
50 MHz	20 dB	10 dBm	-8 dBm	-18 dBm	dBm	0.30 dB	-18 dBm \pm 1.0 dB
50 MHz	10 dB	-10 dBm	-10 dBm	-20 dBm	dBm	0.30 dB	-20 dBm \pm 1.0 dB
50 MHz	10 dB	-10 dBm	-14 dBm	-24 dBm	dBm	0.30 dB	-24 dBm \pm 1.0 dB
50 MHz	10 dB	-10 dBm	-18 dBm	-28 dBm	dBm	0.30 dB	-28 dBm \pm 1.0 dB
50 MHz	0 dB	-20 dBm	-20 dBm	-30 dBm	dBm	0.30 dB	-30 dBm \pm 1.0 dB

Table A-5. MS2070A/80A Power Level Accuracy (Preamplifier On)

Frequency	NRP18T Power Level	MS2070A/80A Expected Power Level	MS2070A/80A Measured Power Level	Measurement Uncertainty	Specification
100 kHz	-10 dBm	-50 dBm	dBm	0.30 dB	-50 dBm \pm 1.0 dB
10 MHz	-10 dBm	-50 dBm	dBm	0.30 dB	-50 dBm \pm 1.0 dB
150 MHz	-10 dBm	-50 dBm	dBm	0.30 dB	-50 dBm \pm 1.0 dB
1 GHz	-10 dBm	-50 dBm	dBm	0.30 dB	-50 dBm \pm 1.0 dB
2.99 GHz	-10 dBm	-50 dBm	dBm	0.30 dB	-50 dBm \pm 1.0 dB
MS2080A-0704					
3.99 GHz	-10 dBm	-50 dBm	dBm	0.30 dB	-50 dBm \pm 1.0 dB
MS2080A-0706					
5 GHz	-10 dBm	-50 dBm	dBm	0.30 dB	-50 dBm \pm 1.0 dB
5.99 GHz	-10 dBm	-50 dBm	dBm	0.30 dB	-50 dBm \pm 1.0 dB

MS2070A/80A Firmware Rev: _____ Operator: _____ Date: _____

Serial Number: _____ Options: _____

Table A-6. MS2070A/80A Spectral Purity - SSB Phase Noise Offset from 1 GHz

Frequency	Measured Delta with 1 kHz RBW	Calculated Value (Measured - 30 dB)	Measurement Uncertainty	Specification (For Calculated Value)
10 kHz	dBc	dBc/Hz	2.0 dB	-93 dBc/Hz max
100 kHz	dBc	dBc/Hz	2.0 dB	-95 dBc/Hz max
1 MHz	dBc	dBc/Hz	2.0 dB	-120 dBc/Hz max

Table A-7. MS2070A/80A Second Harmonic Distortion

Center Frequency	Measured Value	Second Harmonic Distortion (100.2 Meas Value – 50.1 Meas Value)	Measurement Uncertainty	Specification
50.1 MHz	dBm	dBc	1.0 dB	-65 dBc max
100.2 MHz	dBm	dBc	1.0 dB	-70 dBc max

Table A-8. MS2070A Displayed Average Noise Level (Preamplifier Off)

Start Frequency	Stop Frequency	RBW	VBW	Measured Value – 60 dB	Measurement Uncertainty	Specification
10 MHz	2 GHz	1 MHz	1 kHz	dBm	2.0 dB	-142 dBm max
2 GHz	3 GHz	1 MHz	1 kHz	dBm	2.0 dB	-140 dBm max

Table A-9. MS2080A Displayed Average Noise Level (Preamplifier Off)

Start Frequency	Stop Frequency	RBW	VBW	Measured Value – 60 dB	Measurement Uncertainty	Specification
10 MHz	2 GHz	1 MHz	1 kHz	dBm	2.0 dB	-142 dBm max
2 GHz	4 GHz	1 MHz	1 kHz	dBm	2.0 dB	-140 dBm max
4 GHz	5 GHz	1 MHz	1 kHz	dBm	2.0 dB	-137 dBm max
5 GHz	6 GHz	1 MHz	1 kHz	dBm	2.0 dB	-133 dBm max

MS2070A/80A Firmware Rev: _____ Operator: _____ Date: _____

Serial Number: _____ Options: _____

Table A-10. MS2070A Displayed Average Noise Level (Preamplifier On)

Start Frequency	Stop Frequency	RBW	VBW	Measured Value – 60 dB	Measurement Uncertainty	Specification
10 MHz	2 GHz	1 MHz	1 kHz	dBm	2.0 dB	–161 dBm max
2 GHz	3 GHz	1 MHz	1 kHz	dBm	2.0 dB	–160 dBm max

Table A-11. MS2080A Displayed Average Noise Level (Preamplifier On)

Start Frequency	Stop Frequency	RBW	VBW	Measured Value – 60 dB	Measurement Uncertainty	Specification
10 MHz	2 GHz	1 MHz	1 kHz	dBm	2.0 dB	–161 dBm max
2 GHz	4 GHz	1 MHz	1 kHz	dBm	2.0 dB	–160 dBm max
4 GHz	5 GHz	1 MHz	1 kHz	dBm	2.0 dB	–157 dBm max
5 GHz	6 GHz	1 MHz	1 kHz	dBm	2.0 dB	–152 dBm max

Table A-12. MS2070A Residual Spurs (Preamplifier On)

Start Frequency	Stop Frequency	RBW	VBW	Measured Value	Measurement Uncertainty	Specification
10 MHz	500 MHz	300 Hz	100 Hz	dBm	1.4 dB	<–105 dBm, max
500 MHz	1000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<–105 dBm, max
1000 MHz	1500 MHz	300 Hz	100 Hz	dBm	1.4 dB	<–105 dBm, max
1500 MHz	2500 MHz	300 Hz	100 Hz	dBm	1.4 dB	<–105 dBm, max
2500 MHz	3000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<–105 dBm, max

MS2070A/80A Firmware Rev: _____ Operator: _____ Date: _____
 Serial Number: _____ Options: _____

Table A-13. MS2080A Residual Spurs (Preamplifier On)

Start Frequency	Stop Frequency	RBW	VBW	Measured Value	Measurement Uncertainty	Specification
10 MHz	500 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-110 dBm, max
500 MHz	1000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-110 dBm, max
1000 MHz	1500 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-110 dBm, max
1500 MHz	2500 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-110 dBm, max
2500 MHz	3000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-110 dBm, max
3000 MHz	4000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-110 dBm, max
4000 MHz	5000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-110 dBm, max
5000 MHz	6000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-110 dBm, max

Table A-13a. MS2080A Residual Spurs (Preamplifier On, for Rev1 Option 704 models only)

Start Frequency	Stop Frequency	RBW	VBW	Measured Value	Measurement Uncertainty	Specification
10 MHz	500 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-105 dBm, max
500 MHz	1000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-105 dBm, max
1000 MHz	1500 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-105 dBm, max
1500 MHz	2500 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-105 dBm, max
2500 MHz	3000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-105 dBm, max
3000 MHz	4000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-105 dBm, max

Table A-14. MS2070A Residual Spurs (Preamplifier Off)

Start Frequency	Stop Frequency	RBW	VBW	Measured Value	Measurement Uncertainty	Specification
10 MHz	500 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-95 dBm, max
500 MHz	1000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-95 dBm, max
1000 MHz	1500 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-95 dBm, max
1500 MHz	2500 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-95 dBm, max
2500 MHz	3000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-95 dBm, max

MS2070A/80A Firmware Rev: _____ Operator: _____ Date: _____

Serial Number: _____ Options: _____

Table A-15. MS2080A Residual Spurs (Preamplifier Off)

Start Frequency	Stop Frequency	RBW	VBW	Measured Value	Measurement Uncertainty	Specification
10 MHz	500 GHz	300 Hz	100 Hz	dBm	1.4 dB	<-95 dBm, max
500 MHz	1000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-95 dBm, max
1000 MHz	1500 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-95 dBm, max
1500 MHz	2500 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-95 dBm, max
2500 MHz	3000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-95 dBm, max
3000 MHz	4000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-95 dBm, max
4000 MHz	5000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-90 dBm, max
5000 MHz	6000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-90 dBm, max

Table A-15a. MS2080A Residual Spurs (Preamplifier Off, for Rev1 Option 704 models only)

Start Frequency	Stop Frequency	RBW	VBW	Measured Value	Measurement Uncertainty	Specification
10 MHz	500 GHz	300 Hz	100 Hz	dBm	1.4 dB	<-94 dBm, max
500 MHz	1000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-94 dBm, max
1000 MHz	1500 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-94 dBm, max
1500 MHz	2500 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-94 dBm, max
2500 MHz	3000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-94 dBm, max
3000 MHz	4000 MHz	300 Hz	100 Hz	dBm	1.4 dB	<-88 dBm, max

Table A-16. MS2070A Input Related Spurious

Measured Input Signal (2086 MHz)	Measured Spur (400.5 MHz)	Calculated IRS (Input Signal – Spur)	Measurement Uncertainty	Specification
dBm	dBm	dBc	4.0 dB	< -70 dBc

MS2070A/80A Firmware Rev: _____ Operator: _____ Date: _____

Serial Number: _____ Options: _____

Table A-17. MS2080A Input Related Spurs

Measured Input Signal (742 MHz)	Measured Spur (3500.5 MHz)	Calculated IRS (Input Signal – Spur)	Measurement Uncertainty	Specification
dBm	dBm	dBc	4.0 dB	< -70 dBc

Anritsu



 Anritsu utilizes recycled paper and environmentally conscious inks and toner.

Anritsu Company
490 Jarvis Drive
Morgan Hill, CA 95037-2809
USA
<http://www.anritsu.com>