

FieldFox S-Parameter Measurement Uncertainty

N9950A
N9951A
N9952A



This document is an
addendum to the main
FieldFox Data Sheet,

<http://literature.cdn.keysight.com/litweb/pdf/5990-9783EN.pdf>




Corrected Measurement Uncertainty for N9950A/51A/52A


Full 2-port calibration, 85561A 2.92 mm (f) calibration kit, specifications¹

Power level of -15 dBm, 10 Hz IF bandwidth, no averaging, battery saver off, and 60-minute warm-up time. Includes uncertainties due to drift, noise, compression, and dynamic accuracy. Coverage factor of x1 applied to uncertainties, for ease of comparison with other industry handheld analyzers.

Transmission uncertainty (S21, S12)

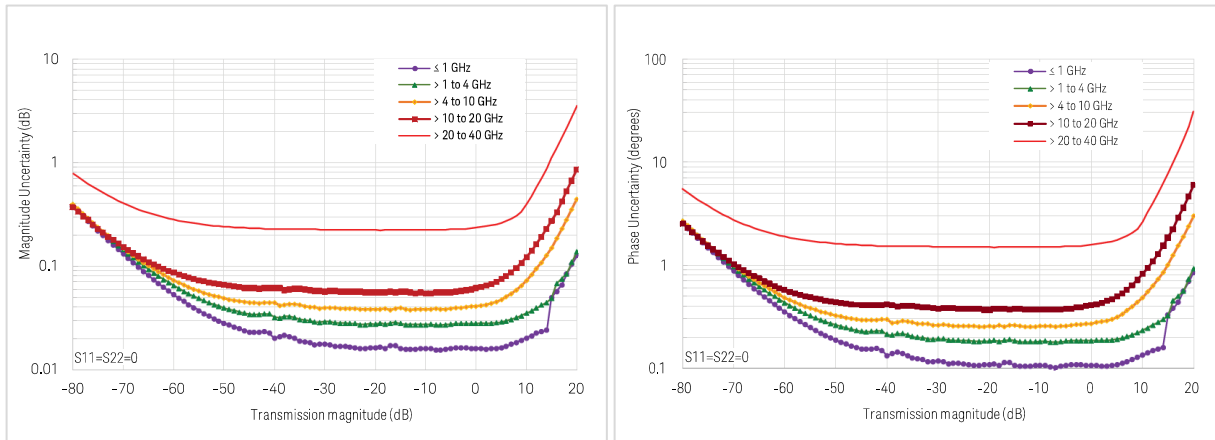

Reflection uncertainty (S11, S22)

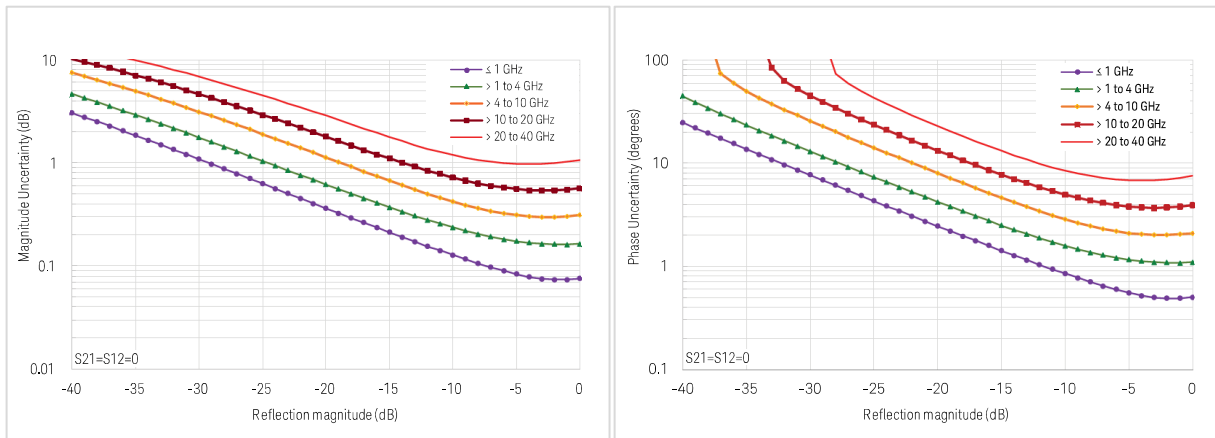


1. Uncertainty curves shown are calculated based on ISO GUM methodology.

Corrected Measurement Uncertainty for N9950A/51A/52A (continued)


Full 2-port calibration, 85562A 2.92 mm (m) calibration kit, specifications¹

Power level of -15 dBm, 10 Hz IF bandwidth, no averaging, battery saver off, and 60-minute warm-up time. Includes uncertainties due to drift, noise, compression, and dynamic accuracy. Coverage factor of x1 applied to uncertainties, for ease of comparison with other industry handheld analyzers.

Transmission uncertainty (S21, S12)

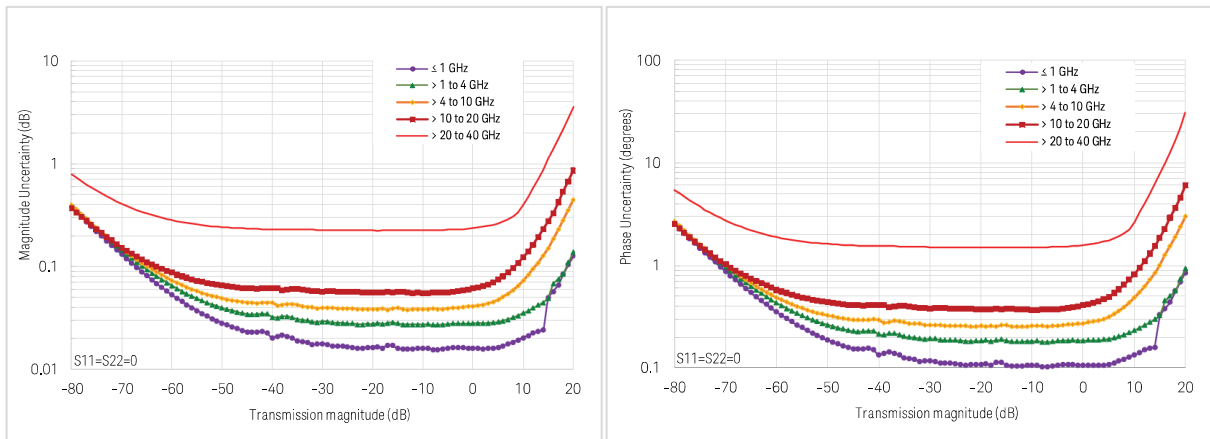

Reflection uncertainty (S11, S22)

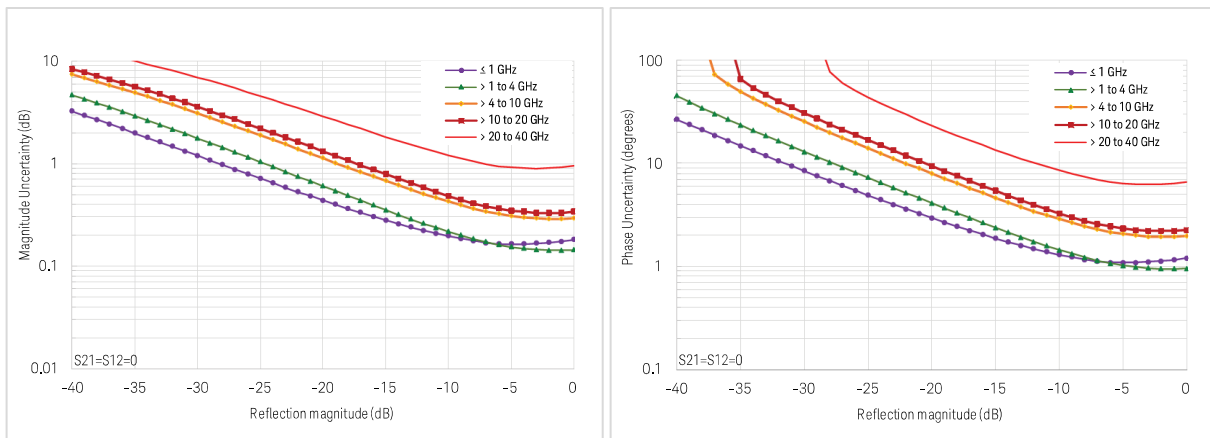


1. Uncertainty curves shown are calculated based on ISO GUM methodology.

Corrected Measurement Uncertainty for N9950A/51A/52A (continued)


Full 2-port calibration, 85563A 2.4 mm (f) calibration kit, specifications¹

Power level of -15 dBm, 10 Hz IF bandwidth, no averaging, battery saver off, and 60-minute warm-up time. Includes uncertainties due to drift, noise, compression, and dynamic accuracy. Coverage factor of x1 applied to uncertainties, for ease of comparison with other industry handheld analyzers.

Transmission uncertainty (S21, S12)

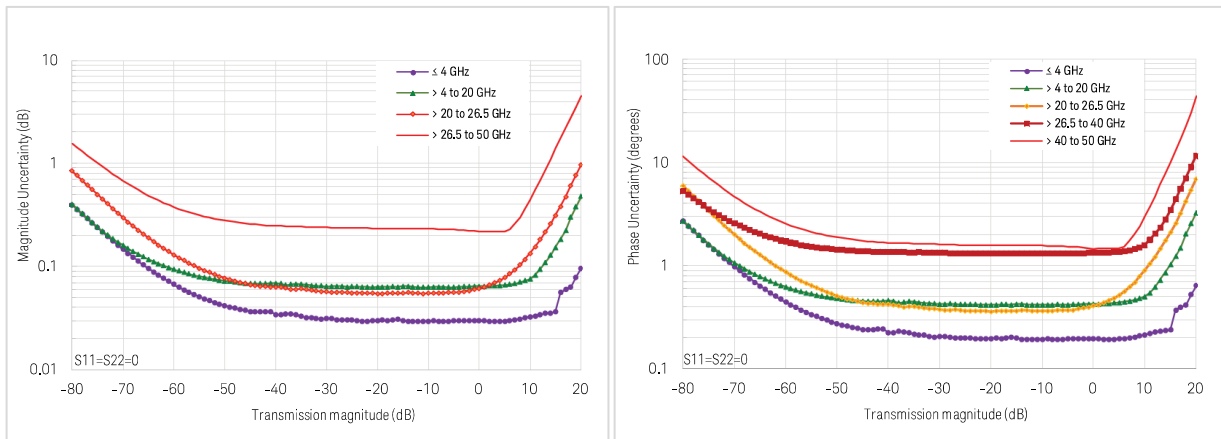

Reflection uncertainty (S11, S22)

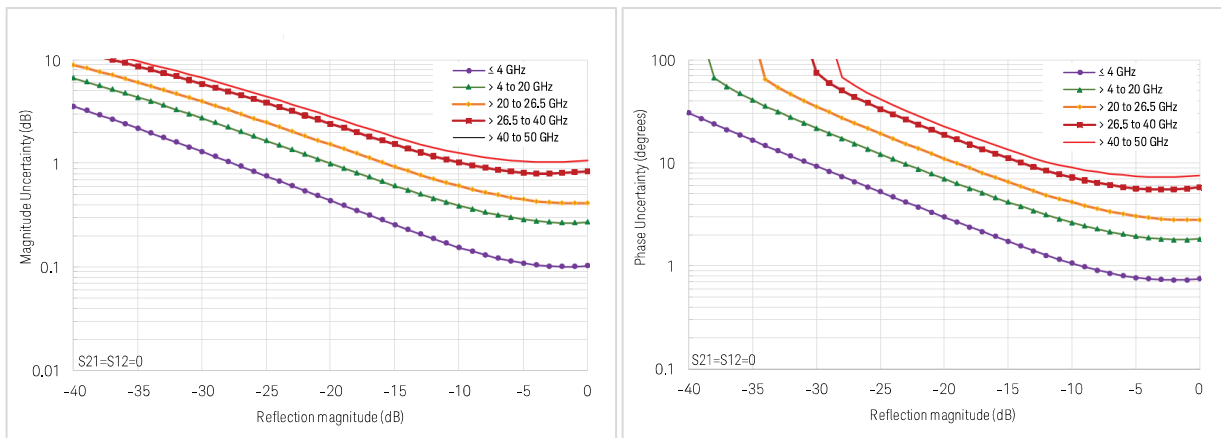


1. Uncertainty curves shown are calculated based on ISO GUM methodology.

Corrected Measurement Uncertainty for N9950A/51A/52A


Full 2-port calibration, 85564A 2.4 mm (m) calibration kit, specifications¹

Power level of -15 dBm, 10 Hz IF bandwidth, no averaging, battery saver off, and 60-minute warm-up time. Includes uncertainties due to drift, noise, compression, and dynamic accuracy. Coverage factor of x1 applied to uncertainties, for ease of comparison with other industry handheld analyzers.

Transmission uncertainty (S21, S12)

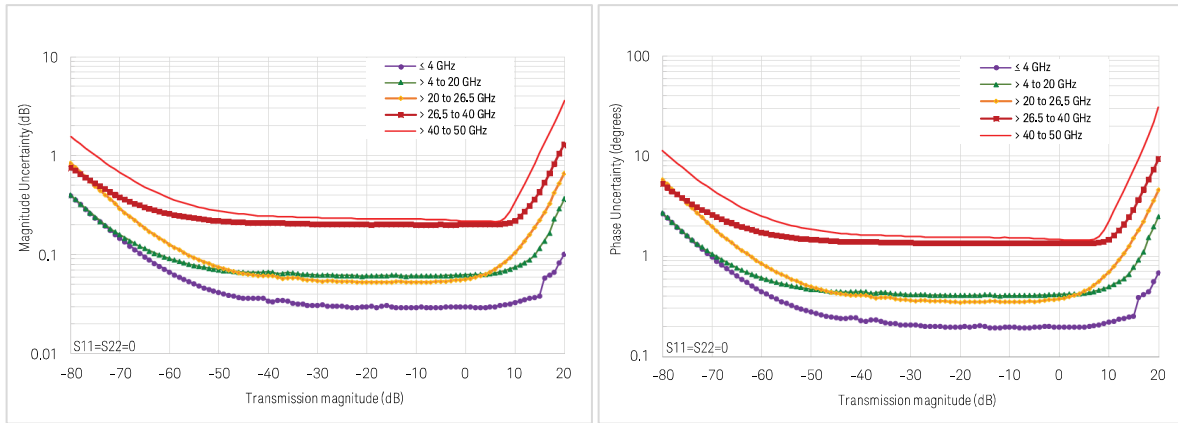

Reflection uncertainty (S11, S22)

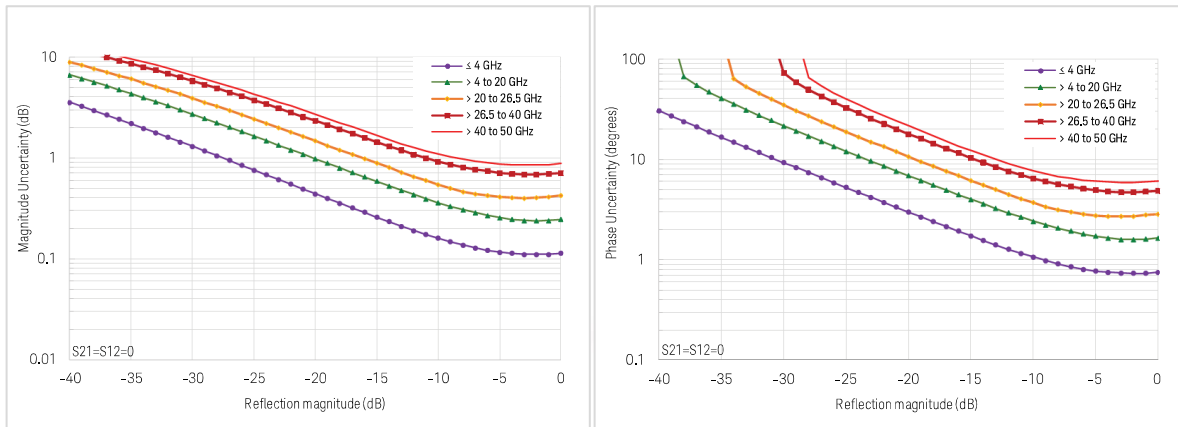

1. Uncertainty curves shown are calculated based on ISO GUM methodology.

Learn more at: www.keysight.com

For more information on Keysight Technologies' products, applications or services, please contact your local Keysight office. The complete list is available at: www.keysight.com/find/contactus

