

Keysight N9911X Economical Waveguide Calibration Components

Configuration
Guide

NOTICE: This document contains references to Agilent Technologies. Agilent's former Test and Measurement business has become Keysight Technologies. For more information, go to www.keysight.com.



Notices

© Keysight Technologies 2013, 2014

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Keysight Technologies as governed by United States and international copyright laws.

Manual Part Number

N9911-90003

Edition

August 2014

Keysight Technologies
1400 Fountaingrove Parkway
Santa Rosa, CA 95403

Warranty

The material contained in this document is provided “as is,” and is subject to being changed, without notice, in future editions. Further, to the maximum extent permitted by applicable law, Keysight disclaims all warranties, either express or implied, with regard to this manual and any information contained herein, including but not limited to the implied warranties of merchantability and fitness for a particular purpose. Keysight shall not be liable for errors or for incidental or consequential damages in connection with the furnishing, use, or performance of this document or of any information contained herein. Should Keysight and the user have a separate written agreement with warranty terms covering the material in this document that conflict with these terms, the warranty terms in the separate agreement shall control.

Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

Restricted Rights Legend

If software is for use in the performance of a U.S. Government prime contract or sub-contract, Software is delivered and licensed as “Commercial computer software” as defined in DFAR 252.227-7014 (June 1995), or as a “commercial item” as defined in FAR 2.101(a) or as “Restricted computer software” as defined in FAR

52.227-19 (June 1987) or any equivalent agency regulation or contract clause. Use, duplication or disclosure of Software is subject to Keysight Technologies’ standard commercial license terms, and non-DOD Departments and Agencies of the U.S. Government will receive no greater than Restricted Rights as defined in FAR 52.227-19(c)(1-2) (June 1987). U.S. Government users will receive no greater than Limited Rights as defined in FAR 52.227-14 (June 1987) or DFAR 252.227-7015 (b)(2) (November 1995), as applicable in any technical data.

Safety Notices

CAUTION

A **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a **CAUTION** notice until the indicated conditions are fully understood and met.

WARNING

A **WARNING** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a **WARNING** notice until the indicated conditions are fully understood and met.

N9911X Economical Waveguide Calibration Components

N9911X Economical Waveguide Calibration Components are used to calibrate Keysight FieldFox Handheld Analyzers. These components are purchased separately — it is not necessary to buy a kit. This allows you to purchase only the components you need, saving the expense of non-necessary components and a storage box.

Use the following information to help determine which N9911X Economical Waveguide Calibration Components to purchase.

Types of Calibration Components

Here is a brief explanation of the types of calibration components that you can purchase. Refer to [“Calibration Component Part Numbers and Photos” on page 3](#) to see images of the components.

Adapter, Waveguide-to-Coax

The adapter is intended for adapting the analyzer’s coaxial connectors to waveguide flanges.

Termination

A termination is also called a load. It is connected directly to the adapter.

$\frac{1}{4}$ Wavelength Offset Shim

A $\frac{1}{4}$ wavelength offset shim is also called a $\frac{1}{4}$ wavelength section. The shim is connected between the adapter and the short to create an **offset short**.

Short

A short is also called a flush short. It is connected directly to the adapter, or used as an **offset short** when combined with the $\frac{1}{4}$ wavelength offset shim.

Coax Cables

To perform a 1-port calibration, one coaxial cable is required. To perform a 2-port calibration, two coaxial cables are required. Each cable is connected between an analyzer test port and a waveguide-to-coax adapter. A list of Keysight cables available for purchase is in the “Accessories” section of the online document *Keysight FieldFox Handheld Analyzers Configuration Guide* (part number 5990-9836EN).

Coupling Set (Hardware) for Flanges

Hardware items such as screws, nuts, washers, and slip pins are necessary for coupling flanges together. One coupling set (english/imperial or metric) contains all of the flange hardware you need for performing both 1-port and 2-port calibrations. It is not necessary to buy more than one coupling set.

Purchasing Calibration Components and Hardware

1. Keysight N9911X Economical Waveguide Calibration Components can be purchased with english/imperial or metric threads. If you already own other Keysight waveguide calibration components, be aware that these have metric threads, so you should order N9911X metric components rather than english/imperial components for full compatibility.
2. To perform a 1-port calibration, you need the following calibration components and hardware. Refer to the tables in ["Calibration Component Part Numbers and Photos" on page 3](#) for part number information.
 - Adapter, qty 1
 - Termination, qty 1
 - Flush short, qty 1
 - 1/4 wavelength offset shim, qty 1
 - Coax cable, qty 1 (refer to ["Coax Cables" on page 1](#))
 - Coupling set, qty 1 (refer to ["Coupling Set \(Hardware\) for Flanges" on page 1](#))
3. To perform a 2-port calibration, you need the following calibration components and hardware. Refer to the tables in ["Calibration Component Part Numbers and Photos" on page 3](#) for part number information.
 - Adapter, qty 2
 - Termination, qty 1
 - Flush short, qty 1
 - 1/4 wavelength offset shim, qty 1
 - Coax cable, qty 2 (refer to ["Coax Cables" on page 1](#))
 - Coupling set, qty 1 (refer to ["Coupling Set \(Hardware\) for Flanges" on page 1](#))
4. Purchase the N9911X Economical Waveguide Calibration Components and hardware by contacting Keysight on the Web at: www.keysight.com/find/assist.

Calibration Component Part Numbers and Photos


The tables on the following pages list the part numbers and descriptions for the N9911X Economical Waveguide Calibration Components. The figures on the following pages show photos of the components.

Table 1 Calibration Components with Waveguide Designators C-Band/WR137/WG14, 5.38 – 8.18 GHz

Description	Keysight Option Number
Calibration Grade Components – Metric	
Adapter, WR137 waveguide to type-N (male) coax	N9911X–110
Termination	N9911X–111
Flush short	N9911X–112
¼ wavelength offset shim	N9911X–113
Coupling set for flange (screw, M5 X 30, qty 16; bolt, M5 X 22 X 12, qty 6; bolt, M5 X 30 X 18.5, qty 8; screw, M5 X 45, qty 8; nut, M5, qty 16; washer, M5, qty 32; slip pin, Ø1/8" X 15 mm, qty 4)	N9911X–114
Calibration Grade Components – English (Imperial)	
Adapter, WR137 waveguide to type-N (male) coax	N9911X–115
Termination	N9911X–116
Flush short	N9911X–117
¼ wavelength offset shim	N9911X–118
Coupling set for flange (screw, #10-32 UNF X 1 1/4", qty 16; screw, #10-32 UNF X 1 3/4", qty 8; screw, #10-32 UNF X 1", qty 8; nut, #10-32 UNF, qty 16; washer, M5, qty 32; slip pin, Ø1/8" X 15 mm, qty 4)	N9911X–119

Figure 1

Calibration Components with Waveguide Designators C-Band/WR137/WG14, 5.38 – 8.18 GHz

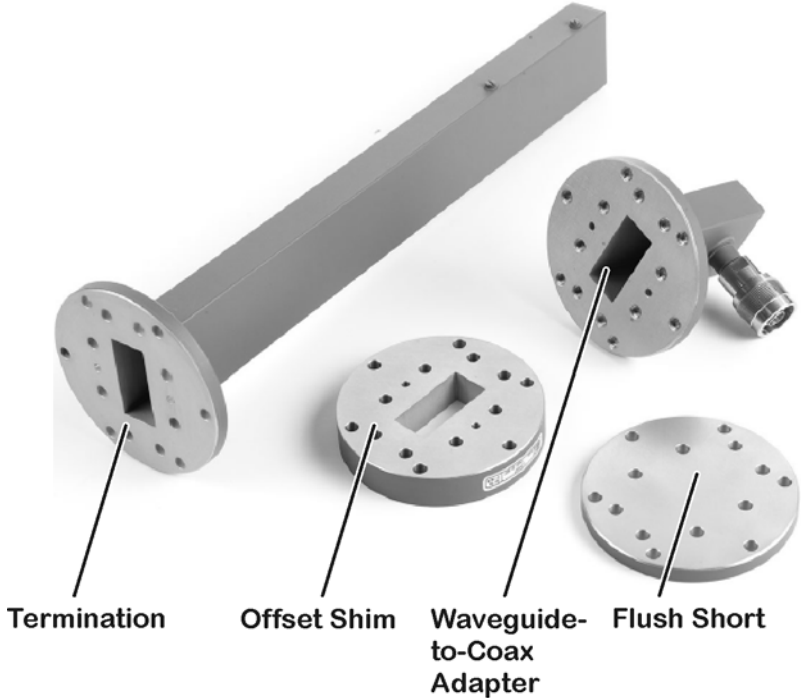


N9911_002_001

Table 2 Calibration Components with Waveguide Designators X-Band/WR90/WG16, 8.2 – 12.5 GHz

Description	Keysight Option Number
Calibration Grade Components – Metric	
Adapter, WR90 waveguide to type-N (male) coax	N9911X–210
Termination	N9911X–211
Flush short	N9911X–212
¼ wavelength offset shim	N9911X–213
Coupling set for flange (screw, M4 X 25, qty 16; screw, M4 X 30, qty 8; bolt, M4 X 21 X 12 (4.0), qty 8; bolt, M4 X 18 X 9 (4.17), qty 4; nut, M4, qty 16; washer, M4, qty 32; slip pin, Ø1/8" X 15 mm, qty 4)	N9911X–214
Calibration Grade Components – English (Imperial)	
Adapter, WR90 waveguide to type-N (male) coax	N9911X–215
Termination	N9911X–216
Flush short	N9911X–217
¼ wavelength offset shim	N9911X–218
Coupling set for flange (screw, #8-32-UNC X 1", qty 16; screw, #8-32 UNC X 1 1/4", qty 8; screw, #8-32 UNC X 3/4", qty 8; nut, #8-32 UNC, qty 16; washer, #8, qty 32; slip pin, Ø1/8" X 15 mm, qty 4)	N9911X–219

Figure 2 Calibration Components with Waveguide Designators X-Band/WR90/WG16, 8.2 – 12.5 GHz

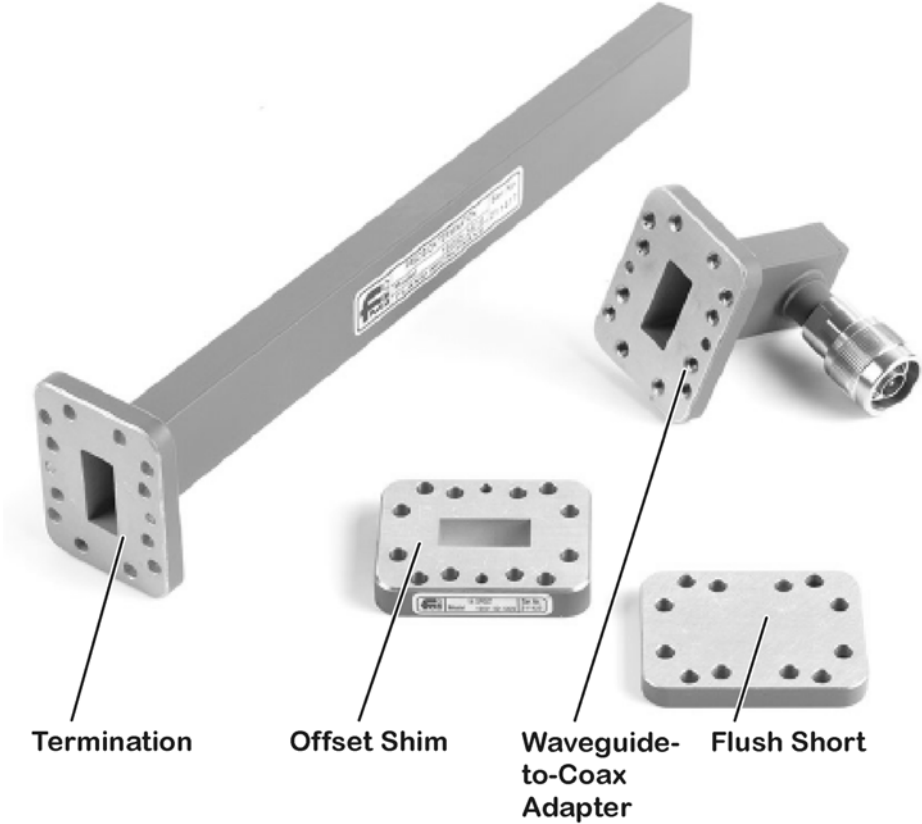


N9911_002_002

Table 3 Calibration Components with Waveguide Designators Ku-Band/WR62/WG18, 11.9 – 18 GHz

Description	Keysight Part Number
Calibration Grade Components – Metric	
Adapter, WR62 waveguide to Type-N (male) coax	N9911X–310
Termination	N9911X–311
Flush short	N9911X–312
¼ wavelength offset shim	N9911X–313
Coupling set for flange (screw, M4 X 25, qty 12; screw, M4 X 30, qty 6; bolt, M4 X 21 X 12 (4.0), qty 6; bolt, M4 x 18 x 9 (4.0), qty 4; nut, M4, qty 12; washer, M4, qty 24; slip pin, Ø1/8" X 15 mm, qty 4)	N9911X–314
Calibration Grade Components – English (Imperial)	
Adapter, WR62 waveguide to Type-N (male) coax	N9911X–315
Termination	N9911X–316
Flush short	N9911X–317
¼ wavelength offset shim	N9911X–318
Coupling set for flange (screw, #6-32-UNC X 1", qty 8; screw, #6-32-UNC X 1 1/4", qty 4; screw, #6-32 UNC X 5/8", qty 4; nut, #6-32 UNC, qty 8; washer, #6, qty 16; slip pin, Ø1/8" X 15 mm, qty 4)	N9911X–319

Figure 3

Calibration Components with Waveguide Designators Ku-Band/WR62/WG18, 11.9 – 18 GHz

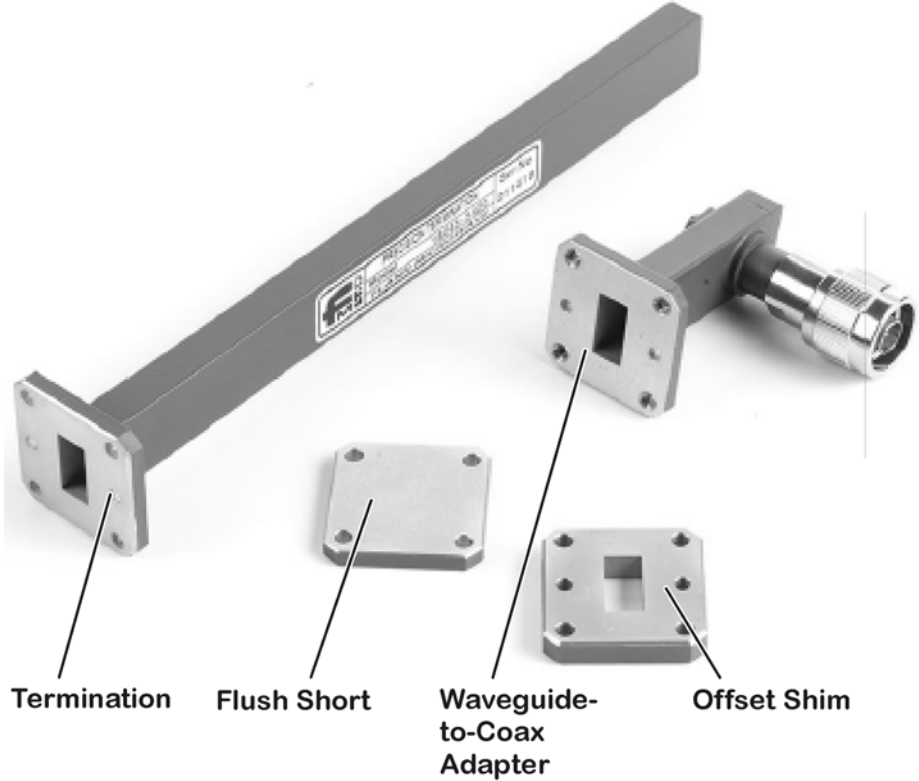

N9911_002_003

Table 4 Calibration Components with Waveguide Designators K-Band/WR42/WG20, 17.6 – 26.7 GHz

Description	Keysight Part Number
Calibration Grade Components – Metric	
Adapter, WR42 waveguide to 3.5 mm (male) coax	N9911X–410
Termination	N9911X–411
Flush short	N9911X–412
$\frac{1}{4}$ wavelength offset shim	N9911X–413
Coupling set for flange (screw, M3 X 20, qty 12; screw, M3 X 25, qty 6; bolt, M3 X 19 X 12.5, qty 6; bolt, M3 X 16 X 10, qty 4; nut, M3, qty 12; washer, M3, qty 24; slip pin, \varnothing 3/32" X 12 mm, qty 4)	N9911X–414
Calibration Grade Components – English (Imperial)	
Adapter, WR 42 waveguide to 3.5 mm (male) coax	N9911X–415
Termination	N9911X–416
Flush short	N9911X–417
$\frac{1}{4}$ wavelength offset shim	N9911X–418
Coupling set for flange (screw, #4-40-UNC X 3/4", qty 8; screw, #4-40 UNX X 1", qty 4; screw, #4-40 UNX X 5/8", qty 4; nut, #4-40 UNC, qty 8; washer, #4, qty 16; slip pin, \varnothing 3/32" X 12 mm, qty 4)	N9911X–419

This information is subject to change without notice.
© Keysight Technologies 2013, 2014
August 2014



N9911-90003
www.keysight.com