Manual for installation tester PCE-ITE 55A / PCE-ITE 55B

07/2023

Table of Contents

1. Preface 4

2. Safety and operational considerations 4

2.1 Warnings and notes 4

2.2 Batteries 7

2.3 Charging 7

2.4 Precautions on charging of new battery cells or cells unused for a longer period 7

2.5. Standards applied 8

3. Instrument description 9

3.1. Front panel (depends on model) 9

3.2. Connector panel (depends on model) 10

3.3. Back panel 10

3.4. Bottom view – Information label 12

3.5. Carrying the instrument 12

4. Instrument operation 13

4.1. Meaning of symbols and messages on the Instrument display 13

4.2. The online voltage and output terminal monitor 14

4.3. Message field – battery status 14

4.4. Status field – measurement warnings/results symbols 15

4.5. Sound warnings 15

4.6. Performing measurement 16

4.6.1. Measurement function/sub-function 16

4.6.2. Selecting measurement function/sub-function 16

4.6.3. Performing tests 16

4.7. Setup menu 16

4.8. Help screen 17

5 Measurements 18

5.1 Insulation resistance 18

5.2 Continuity 19

5.2.1 R low test 19

5.2.2 Continuity test 22

5.3 Testing RCDs 24

5.3.1 Limit contact voltage 24

5.3.2 Nominal differential trip-out current 24

5.3.3 Multiplier of nominal residual current 24

5.3.4 RCD type and test current starting polarity 24

5.3.5 Testing selective (time-delayed) RCDs 25
5.3.6 Contact voltage 25
5.3.7 Trip-out time 27
5.3.8 Trip-out current 29
5.3.9 Autotest 31
5.3.9.1 How to perform RCD autotest 31
5.3.10 WARNINGS 36
5.4 Fault loop impedance and prospective fault current 36
5.4.1 Fault loop impedance 36
5.4.2 The fault loop impedance test RCD (for RCD protected circuits) 38
5.4.3 The fault loop impedance test Rs (for adjustable current) 40
5.5 Line impedance and prospective short-circuit current 41
5.5.1 Voltage drop test 43
5.6 Phase sequence testing 46
5.7 Voltage and frequency 47
5.8 Earth Resistance 49
5.8.1. Earth Resistance (Re) - 3-wire, 4wire 49
5.8.2. Specific earth resistance (Ro) 51
6 Maintenance 53
6.1. Replacing fuses 53
6.2. Cleaning 53
6.3. Periodic calibration 53
6.4. Service 53
6.5. Batteries 54
7 Technical specifications 55
7.1 Insulation resistance 55
7.2 Continuity resistance 55
7.2.1 Low R (depends on model) 55
7.2.2 Low current continuity 56
7.3 RCD testing 56
7.3.1 General data 56
7.3.2 Contact voltage 57
7.3.3 Trip-out time 57
7.3.4 Trip-out current 57
7.4 Fault loop impedance and prospective fault current 58
7.5 Line impedance and prospective short-circuit current 59
7.6 Phase rotation 59

7.7 Voltage and frequency 59
7.8 Earth Resistance 60
7.9 General data 61

1. Preface

Congratulations on your purchase of the PCE-ITE 55 SERIESinstrument and its accessories from PCE Instruments.
The instrument design is based on big company experience, acquired through many years of dealing with electric installation test equipment.
The PCE-ITE 55 SERIESinstrument is a professional, multifunctional, hand-held test instrument intended to perform all the measurements required for verification of electrical safety of installations in buildings.

The following measurements and tests can be performed:

- Continuity tests,
- Insulation resistance tests,
- RCD testing,
- Line / Loop impedance (with Loop RCD option) measurements,
- Voltage and frequency,
- Phase rotation,
- Earth resistance (optional)
- EVSE measurements (optional)

The large TFT colour display with backlight offers easy to read results, indications, measurement parameters and messages. The operation of the instrument is designed to be as simple and clear as possible and no special training (reading this instruction manual would be sufficient) is required in order to begin using the instrument.
The instrument is equipped with all accessories required in order to perform testing comfortably. The soft carrying bag, included with the meter, protects the instrument and keeps all accessories together making it simple and easy to move between locations.

2. Safety and operational considerations

2.1 Warnings and notes

To maintain the highest level of operator safety while carrying out various tests and measurements, PCE Instruments strongly recommends keeping your PCE-ITE 55 SERIESinstruments in best possible condition and undamaged. When using the instrument, consider the following general warnings:

- **The symbol means »Mark on your equipment certifies that it meets requirements of all subjected EU regulations. «**
- **The symbol means »This equipment should be recycled as electronic waste. «**
- **The symbol on the instrument means »Read the Instruction manual with special care for safe operation«. The symbol requires an action!**
- **The symbol means »Danger: risk of high voltage! «**
- **The symbol means »Class II: Double Insulated«. No need for safety connection to Earth.**

- **If the test equipment is used in a manner not specified in this user manual, the protection provided by the equipment could be impaired!**
- **Read this user manual carefully, otherwise the use of the instrument may be dangerous for the operator, the instrument or for the equipment under test!**
- **Stop using the instrument or any of the accessories if any damage is noticed!**
- **If a fuse blows in the instrument, follow the instructions in this manual in order to replace it!**
- **Consider all generally known precautions in order to avoid risk of electric shock while dealing with hazardous voltages!**
- **Do not use the instrument in supply systems with voltages higher than 550 V!**
- **Service intervention or adjustment is only allowed to be carried out by competent authorized personnel!**
- **Use only standard or optional test accessories supplied by your distributor!**
- **The instrument comes supplied with rechargeable Ni-MH battery cells. The cells should only be replaced with the same type as defined on the battery compartment label or as described in this manual. Do not use standard alkaline battery cells while the power supply adapter is connected, otherwise they may explode!**
- **Hazardous voltages exist inside the instrument. Disconnect all test leads, remove the power supply cable and switch off the instrument before removing battery compartment cover.**
- **All normal safety precautions must be taken in order to avoid risk of electric shock while working on electrical installations!**

⚠ Warnings related to measurement functions

Insulation resistance

- Insulation resistance measurement should only be performed on de-energized objects!
- When measuring the insulation resistance between installation conductors, all loads must be disconnected, and all switches closed!
- Do not touch the test object during the measurement or before it is fully discharged! Risk of electric shock!
- Do not connect test terminals to external voltage higher than 550 V (AC or DC) in order not to damage the test instrument!

Continuity functions

- Continuity measurements should only be performed on de-energized objects!
- Parallel impedances or transient currents may influence test results.

Testing PE terminal

- If phase voltage is detected on the tested PE terminal, stop all measurements immediately and ensure the cause of the fault is eliminated before proceeding with any activity!

Notes related to measurement functions

General

- The **"!"** indicator means that the selected measurement cannot be performed because of irregular conditions on input terminals.
- Insulation resistance, continuity functions and earth resistance measurements can only be performed on de-energized objects.
- PASS / FAIL indication is enabled when limit is set. Apply appropriate limit value for evaluation of measurement results.
- In the case that only two of the three wires are connected to the electrical installation under test, only voltage indication between these two wires is valid.

Insulation resistance

- If voltages of higher than 10 V (AC or DC) are detected between test terminals, the insulation resistance measurement will not be performed.

Continuity functions

- If voltages of higher than 10 V (AC or DC) are detected between test terminals, the continuity resistance test will not be performed.
- Before performing a continuity measurement, where necessary, compensate test lead resistance.

RCD functions

- Parameters set in one function are also kept for other RCD functions!
- The measurement of contact voltage does not normally trip an RCD. However, the trip limit of the RCD may be exceeded because of leakage current flowing to the PE protective conductor or a capacitive connection between L and PE conductors.
- The RCD trip-lock sub-function (function selector switch in **LOOP** position) takes longer to complete but offers much better accuracy of fault loop resistance (in comparison to the R_L sub-result in **Contact voltage** function).
- RCD trip-out time and RCD trip-out current measurements will only be performed if the contact voltage in the pre-test at nominal differential current is lower than the set contact voltage limit!
- The auto-test sequence (RCD AUTO function) stops when trip-out time is out of allowable time period.

Loop impedance (with Loop RCD and / or Loop Rs option)

- Isc depends on Z, Un and scaling factor
- The current limit depends on fuse type, fuse current rating, fuse trip-out time
- The specified accuracy of tested parameters is valid only if the mains voltage is stable during the measurement.
- Fault loop impedance measurements will trip an RCD.
- The measurement of fault loop impedance using trip-lock function does not normally trip an RCD. However, the trip limit may be exceeded as a result of leakage current flowing to the PE protective conductor or a capacitive connection between L and PE conductors.

Line impedance

- Isc depends on Z, Un and scaling factor

- The current limit depends on fuse type, fuse current rating, fuse trip-out time
- The specified accuracy of tested parameters is valid only if the mains voltage is stable during the measurement.

2.2 Batteries

⚠

When connected to an installation, the instruments battery compartment can contain hazardous voltage inside! When replacing battery cells or before opening the battery/fuse compartment cover, disconnect any measuring accessory connected to the instrument and turn off the instrument,

- Ensure that the battery cells are inserted correctly otherwise the instrument will not operate and the batteries could be discharged.
- If the instrument is not to be used for a long period of time, remove all batteries from the battery compartment.
- Rechargeable Ni-MH batteries (size AA) can be used. It is recommended only using of rechargeable batteries with a capacity of 2300mAh or above.
- Do not recharge alkaline battery cells!

2.3 Charging

The batteries will begin charging whenever the power supply adapter is connected to the instrument. The built-in protection circuits control the charging procedure and assure maximum battery lifetime. The power supply socket polarity is shown in figure 2.1.

Figure 2.1: Power supply socket polarity

Note:

Use only power supply adapter delivered from the manufacturer or distributor of the test equipment to avoid possible fire or electric shock!

2.4 Precautions on charging of new battery cells or cells unused for a longer period

Unpredictable chemical processes can occur during the charging of new battery cells or cells that have been left unused for long periods of time (more than 3 months).

When using an external intelligent battery charger, one complete discharging/charging cycle can be performed automatically. After performing this procedure, a normal battery capacity should be fully restored, and the operating time of the instrument will approximately meet the data set out in the in the technical specification.

Notes:

- The charger in the instrument is a pack cell charger. This means that the cells are connected in series during the charging so all of them must be in similar state

(similarly charged, same type and age).

- If even one deteriorated battery cell (or just one of a different type e.g. capacity, chemical design) can cause disrupted charging of the entire battery pack which could lead to overheating of the battery pack and a significant decrease in the operating time.
- If no improvement is achieved after performing several charging/discharging cycles, the state of each individual battery cells should be determined (by comparing battery voltages, checking them in a cell charger, etc). It is very likely that one or more of the battery cells could have deteriorated.
- The effects described above should not be mixed with the normal battery capacity decrease over time. All charging batteries lose some of their capacity when repeatedly charged/discharged. The actual decrease in capacity compared to the number of charging cycles depends on the battery type. This information is normally provided in the technical specification from battery manufacturer.

2.5. Standards applied

The PCE-ITE 55 SERIESinstrument is manufactured and tested in accordance with the following regulations:

Electromagnetic compatibility (EMC)	
EN 61326	Electrical equipment for measurement, control and laboratory use – EMC requirements Class B (Hand-held equipment used in controlled EM environments)
Safety (LVD)	
EN 61010-1	Safety requirements for electrical equipment for measurement, control and laboratory use – Part 1: General requirements
EN 61010-031	Safety requirements for hand-held probe assemblies for electrical measurement and test
Functionality	
EN 61557	Electrical safety in low voltage distribution systems up to 1000 V_{AC} and 1500 V_{AC} – Equipment for testing, measuring or monitoring of protective measures Part 1.....General requirements Part 2.....Insulation resistance Part 3.....Loop resistance Part 4.....Resistance of earth connection and equipotential bonding Part 5.....Resistance to earth Part 6.....Residual current devices (RCDs) in TT and TN systems Part 7.....Phase sequence Part 10.....Combined measuring equipment
DIN VDE 0100	
EVSE	
IEC 62955	Residual direct current detecting device (RDC-DD) to be used for mode 3 charging of electric vehicles

Note about EN and IEC standards:

- Text of this manual contains references to European standards. All standards of EN 6XXXX (e.g. EN 61010) series are equivalent to IEC standards with the same number (e.g. IEC 61010) and differ only in amended parts required by European harmonization procedure.

3. Instrument description

3.1. Front panel (depends on model)

Figure 3.1: Front panel

Legend:

1 - Function selector switch

2 - Setup key

3 - Exit/Back/Return key

4 - ON/OFF key, to switch the instrument on and off. The instrument will automatically switch off (APO) after the last key press and no voltage is applied.

5 - Memory key

6 - Compensation key, to compensate for the test lead resistance in low-value resistance measurements

7 - Help key

8 - Up and down keys

9 - Left and right keys

10 - TEST key for starting / confirmation tests

11 - TFT color display

3.2. Connector panel (depends on model)

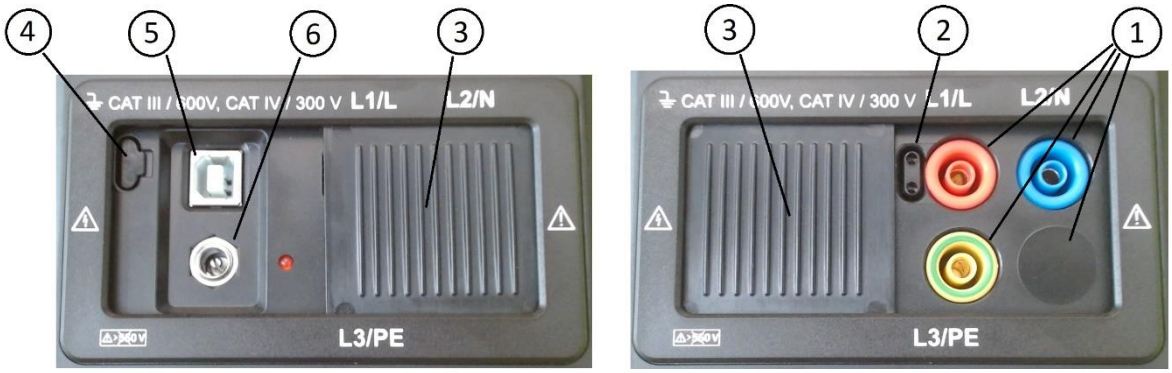

Figure 3.2: Connector panel

Legend:

1 - Test connector.
Warning! Maximum allowed voltage between test terminals and ground is 600V!
Maximal allowed voltage between test terminals is 550 V!

2 - Socket for probe with Test push button

3 - Protection cover above USB-B connector

4- USB 3 connector. (depends on model)

5- USB B connector for data transfer (depends on model)

6 - Battery charger input (depends on model)

3.3. Back panel

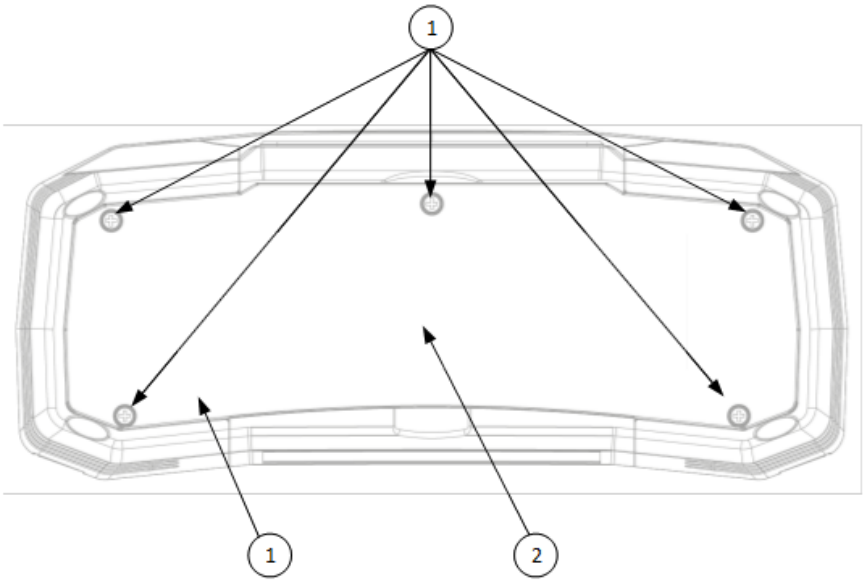

Figure 3.3: Back panel

Legend:

1 - Battery/fuse compartment cover.

2 - Information label.

3 - Fixing screws for battery/fuse compartment cover.

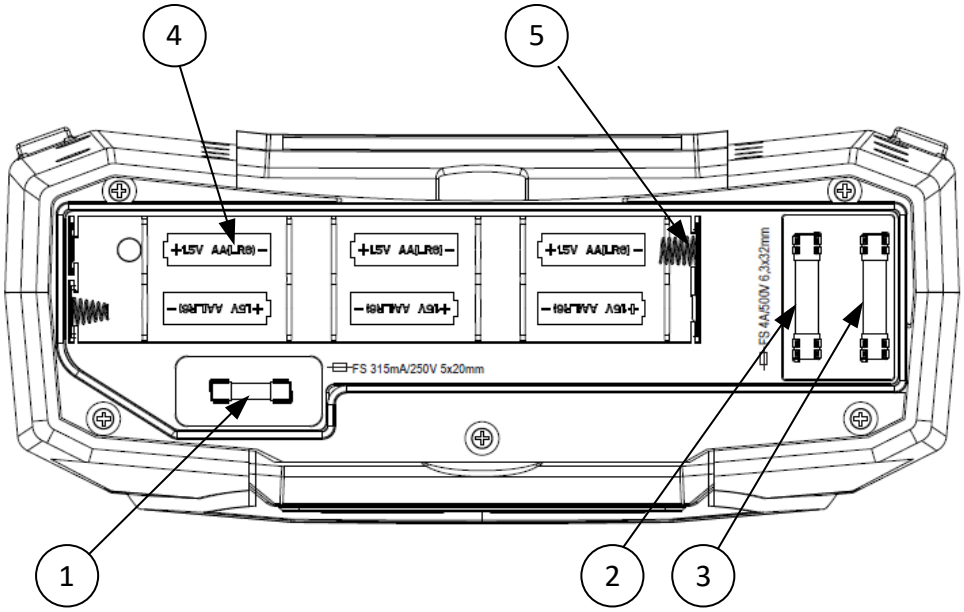

Figure 3.4.: *Battery and fuse compartment*

Legend:

1.....Fuse F3.

2.....Fuse F2.

3.....Fuse F1.

4 ..... Battery cells (size AA).

5 ..... Battery contacts.

3.4. Bottom view – Information label

Function	EN61557	range	Accuracy	
Continuity	-4	0.1 Ω ... 20.0 Ω 0.1 Ω ... 1999 Ω	±(3% of read. + 3 digits) ±(5% of read. + 3 digits)	Test current min. 200mA at 2 Ohm Test current max. 7 mA Open circuit voltage 5V
Insulation resistance	-2	0.1 MΩ ... 199.9 MΩ 0.1 MΩ ... 199.9 MΩ 200 MΩ ... 999 MΩ	±(5% of read. + 3 digits) ±(2% of read. + 3 digits) ±(10% of read.)	50/100/250V 500/1000V max. 15mA
RCD Time Current Contact voltage	-6	0.0 ... 500ms 0.2xIΔN ... 1.1xIΔN (AC) 0.2xIΔN ... 1.5xIΔN (A), (IΔN ≥30 mA) 0.2xIΔN ... 2.2xIΔN (A), (IΔN <30 mA) 0.2xIΔN ... 2.2xIΔN (B) 3V ... 99.9V	±3ms ±0.1xIΔN (-0%/±10%) of read.±5 digits	IΔN 6,10,30,100,300, 500,650,1000mA
Impedance	-3	0.25 Ω ... 9999 Ω 0.25 Ω ... 9999 Ω 0.75 Ω ... 19.99 Ω 20 Ω ... 9999 Ω	±(5% of read. + 5 digits) ±(5% of read. + 5 digits) ±(5% of read. + 10 digits) ±(10% of read.)	Z line L-L,L-N Z loop L-PE Z loop L-PE non-trip Line: 93V-134V; 185V-266V; 321V-485V; 45Hz-65Hz Loop: 93V-134V; 185V-266V; 45Hz-65Hz
Voltage Frequency	-7	0 ... 550V (45-400Hz) 10.0 ... 499.9Hz	±(2% of read. + 2 digits) ±(0.2% + 1digits)	TRMS
Phase rotation	-7	50 ... 550VAC 45 ... 400Hz		Right:1-2-3 Left:3-2-1
Earth resistance	-5	1.0 Ω ... 9999 Ω 6.0 Ω ... 9999 Ω	±(5% of read. + 5 digits)	3-wire, 4-wire Specific earth resistance f=126.9Hz

Figure 3.5: Bottom panel information label

3.5. Carrying the instrument

The neck strap supplied in standard set allows the instrument to be carried in a variety of different ways. The operator can choose the most appropriate method based on the tasks they are performing.

The instrument can be hung around operator's neck allowing the instrument to move freely. This allows equipment to be moved quickly between test locations.

4. Instrument operation

4.1. Meaning of symbols and messages on the Instrument display

The instrument display is divided into several sections:

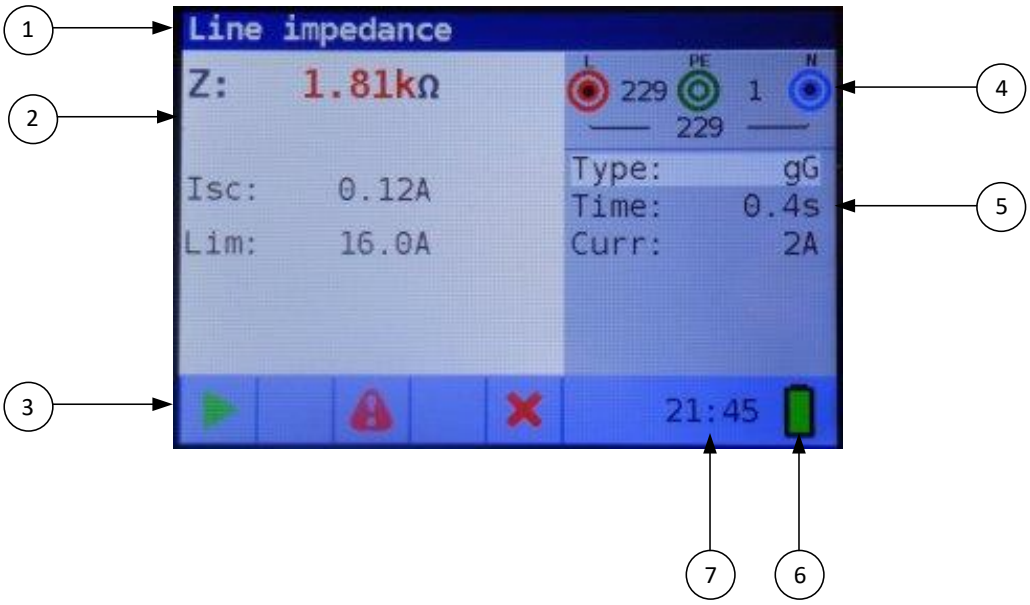

Figure 4.1: Display outlook

Legend:

1 - Function line.
2 - Result field.
In this field the main result and sub-results are displayed.
3 - Status field
PASS/FAIL/ABORT/START/WAIT/WARNINGS status are displayed.
4 - Online voltage and output monitor.
Shows symbolized plugs, names the plugs depending on the measurements, always shows the actual voltages.
5 - Options field
6 - Battery status indication
7 - Current time

4.2. The online voltage and output terminal monitor

Online voltages are displayed together with test terminal indication. All three test terminals are used for selected measurement.

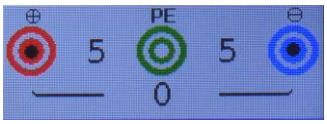

Online voltages are displayed together with test terminal indication. L and N test terminals are used for selected measurement.

4.3. Message field – battery status

Battery power indication.

Low battery indication. Battery pack is too weak to guarantee correct result. Replace the batteries.

Recharging is shown by a LED near the supply socket.

4.4.Status field – measurement warnings/results symbols

Symbol	Meaning	Active in function:											
		Voltage Rotation	R low	Continuity	R Isolation	Line	Loop	Loop RCD	RCD time	RCD current	RCD auto	RCD Uc	Earth resistance
	Dangerous voltage	X	X	X	X	X	X	X	X	X	X	X	X
COMP	Test leads are compensated		X	X									
	Measurement cannot be started		X	X	X								
	Dangerous voltage on PE	X	X	X	X	X	X	X	X	X	X	X	X
	Result is not ok		X	X	X	X	X	X	X	X	X	X	X
	Result is ok		X	X	X	X	X	X	X	X	X	X	X
	RCD open or tripped								X	X	X	X	
	RCD closed								X	X	X	X	
	Measurement can be started		X	X	X	X	X	X	X	X	X	X	X
	Temperature too high					X	X	X	X	X	X	X	
	Swap test leads	X	X	X	X	X	X	X	X	X	X	X	X
	Wait				X								
	Noise on signal					X	X	X	X	X	X	X	
	Check fuses		X	X	X								X
REF	Reference measurement (optional)					X							
SF	Single fault in IT system (optional)	X				X	X	X	X	X	X	X	

Figure 4-1 List of status symbols

4.5.Sound warnings

Short high sound	button pressed
continued sound	during continuity test when result is <35 Ohm
upwards sound	attention, dangerous voltage applied
Short sound	power off, end of measurement
downwards sound	warnings (temperature, voltage at input, start not possible)

Periodic sound	**Warning!** Phase voltage on the PE terminal! Stop all the measurements immediately and eliminate the fault before proceeding with any activity!

4.6. Performing measurement

4.6.1. Measurement function/ sub-function

The following measurements can be selected with the function selector switch:

- Voltage/rotation/frequency measurement
- Earth resistance
- R Low
- R Insulation
- Line impedance
- Loop (Loop RCD) impedance
- RCD
- EVSE measurement (option)

The function/sub-function name is highlighted on the display by default.

4.6.2. Selecting measurement function/ sub-function

Using navigation keys ▲▼ select the parameter/limit value you want to edit. By using ◀▶ keys the value for the selected parameter can be set.
Once the measurement parameters are set, the settings are retained until new changes are made.

4.6.3. Performing tests

When ▶ symbol is displayed test can be started by pressing the “TEST” button. After completion of the test its result value and status will be displayed. In case of PASSED measurement, result value will be displayed in black color along with the ✓ status symbol. In case of NOT PASSED measurement, the result value will be marked in red color along with the ✖ symbol.

4.7. Setup menu

To enter the **Setup** menu, press the SETUP key. In the **Setup** menu, the following actions can be taken:

- Isc factor:

  Set prospective short/fault current scaling factor

- Date/Time:

  Set internal date and time

  Calibration date (optional)

- RCD standard:

  Select national standard for RCD testing, e.g EN61008 or BS7671

- ELV:

  Select voltage for ELV warning.

- Power off time:

  Select time when device should switch off if not used.

- Cont timeout:

  Select time-out when measurement should stop automatically.

- ISO timeout:

  Select time-out when measurement should stop automatically.

- Supply system:

  Select supply network/system, e.g. TN or IT.

- Device info:

  Shows info about device, e.g. Firmware version

- Language:

  Set the language

- Buzzer:

  Set the options, when the buzzer should be active

- Backlight:

  Set the level of the TFT display backlight

4.8. Help screen

The Help screens contain diagrams that show the correct use of the device.

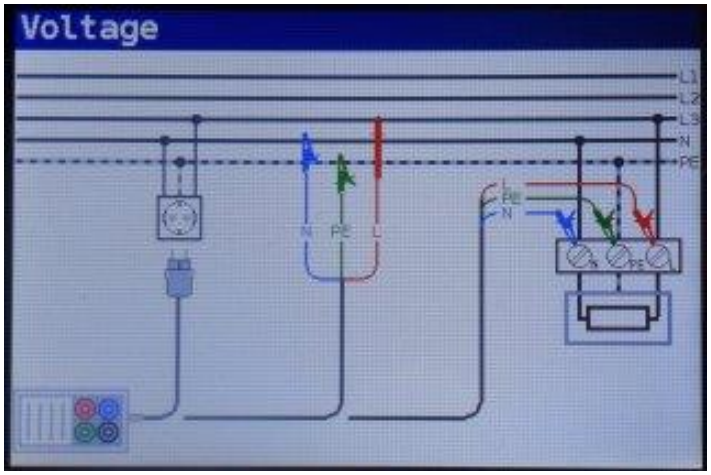

Figure 4-8: example of a help screen

Press the HLP key to enter the help screen
Press the HLP key or the Exit/Back/Return key to exit the help screen
Press the Left and Right keys to switch to previous/next help screen

5 Measurements

5.1 Insulation resistance

The Insulation resistance measurement is performed in order to ensure safety against electric shock. Using this measurement, the following items can be determined:

- Insulation resistance between installation conductors,
- Insulation resistance of non-conductive rooms (walls and floors),
- Insulation resistance of ground cables,
- Resistance of semi-conductive (antistatic) floors.

How to perform an insulation resistance measurement

Step 1 Select **Insulation** function with the function selector switch. The following menu is displayed:

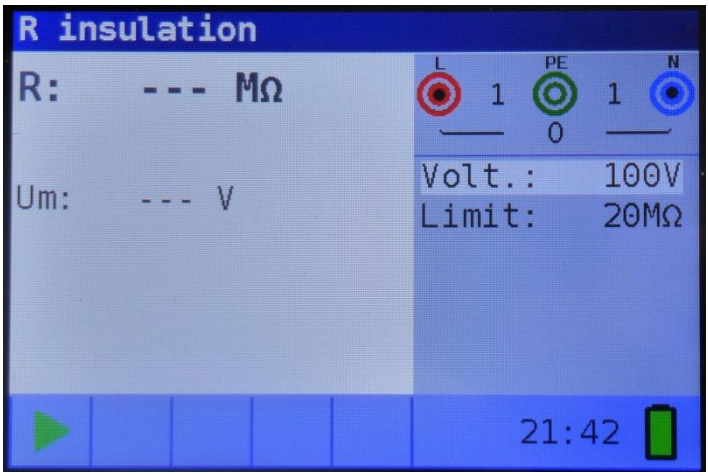

Figure 5-1: Insulation resistance measurement menu

Step 2 Set the following measuring parameter and limit values:

- **Volt:** Nominal test voltage,
- **Limit:** Low limit resistance value.

Step 3 Ensure that no voltages are present on the item for testing. Connect the test leads to the PCE-ITE 55 SERIESinstrument. Connect the test cables to the item under test. (see figure 5.2) to perform insulation resistance measurement.

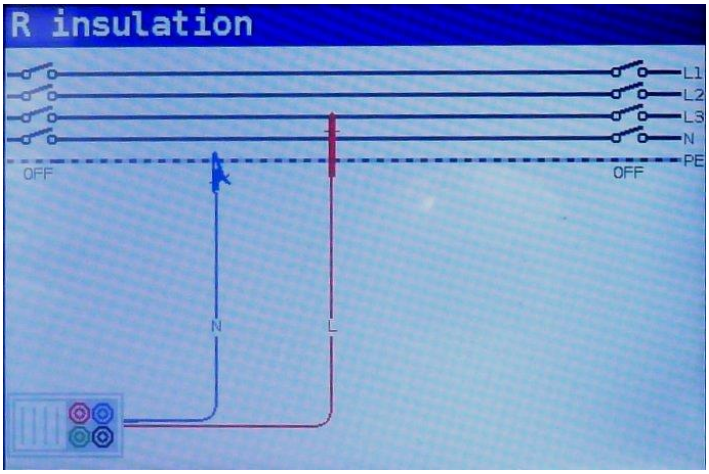

Figure 5-2: Connection of universal test cable

Step 4 Check the displayed warnings and online voltage/terminal monitor before starting the measurement. If ▶ is displayed, press the TEST key.
After the test is done, measured results are displayed, together with the e ✔ or ✖ indication (if applicable).

Figure 5-3: Example of insulation resistance measurement results

Displayed results:

R ..... Insulation resistance,
Um ..... Actual voltage applied to item under test

Warnings:

- Insulation resistance measurement should only be performed on de-energized objects!
- When measuring the insulation resistance between installation conductors, all loads must be disconnected and all switches closed!
- Do not touch the test object during the measurement or before it is fully discharged! Risk of electric shock!
- In order to prevent damaging the test instrument, do not connect test terminals to an external voltage higher than 550 V (AC or DC).

5.2 Continuity

Two continuity sub-functions are available:

- R Low, ca. 240mA continuity test with automatic polarity reversal.
- Low current (ca. 4mA) continuous continuity test (optional), useful when testing inductive systems.

5.2.1 R low test

This function is used to test the resistance between two different points of the installation to ensure that a conductive path exists between them. The test ensures that all protective conductors, earth conductors or bonding conductors are correctly connected, terminated and have the correct resistive value.
The measurement of the R Low resistance is performed with a test current of more than 200m@2Ohm. An automatic pole reversal of the test voltage and the test current is performed

during the test. This test checks for any components (e.g. diodes, transistors, SCRs) that may have a rectifying effect on the circuit which could cause problems when a voltage is applied.

This measurement completely complies with EN61557- 4 regulations.

How to perform a R Low resistance measurement

Step 1 Select the **Continuity** function with the function selector switch and select the R Low mode with the ▲▼ and ◄►navigation keys. The following menu will be displayed:

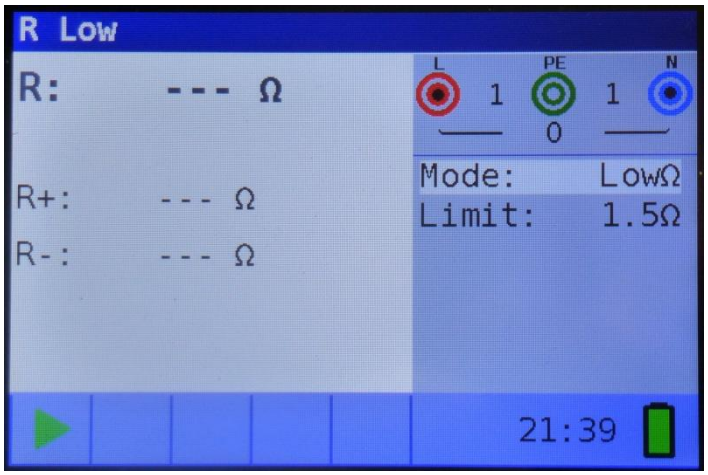

Figure 5-4: R Low resistance measurement menu

Step 2 Set the following limit value:

- **Limit:** limit resistance value using the ▲▼ and ◄►navigation keys.

Step 3 Connect test cable to the PCE-ITE 55 SERIESinstrument. Before performing an R Low resistance measurement, compensate for the test leads resistance as follows:

1. Short test leads first as shown in figure 5.5.



Figure 5-5: Shorted test leads

2 Press the COM key. After performing test leads compensation the compensated test leads indicator **COMP** will be displayed in the status line.

2. In order to remove any test lead resistance compensation, just press the COM key again. After removing any test lead compensation, the compensation indicator will disappear from the status line.

Step 4 Ensure that the item for testing is disconnected from any voltage source and it has been fully discharged. Connect the test cables to the item under test.
Follow the connection diagrams shown in figures 5.6 and 5.7 to perform a R Low resistance measurement.

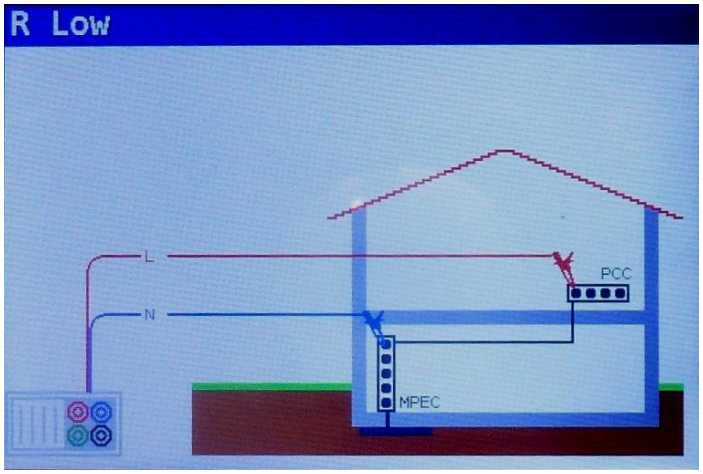

Figure 5-6: Connection of universal test cable

Step 5 Check for any warnings and the online voltage/terminal monitor on the display before starting the measurement. If everything is ok and the ↄ is shown, press the TEST key.
After performing the measurement, the results appear on the display together with the ✎ or ✖ indication (if applicable).

Figure 5-7: Examples of R Low resistance measurement results

Displayed results:
R ..... Main LowΩ resistance result (average of R+ and R- results),
R+ ..... LowΩ resistance sub-result with positive voltage at Lterminal,
R- ..... LowΩ resistance sub-result with positive voltage at Nterminal.

Warnings:

- Low-value resistance measurements should only be performed on de-energized objects!
- Parallel impedances or transient currents may influence test results.

Note:

- If voltage between test terminals is higher than 10 V the R Low measurement will not be performed**.**

5.2.2 Continuity test

Continuous low-value resistance measurements can be performed without pole reversal of the test voltages and a lower test current (a few mA). In general, the function serves as an ordinary Ω-meter with low-test current. The function can also be used to test inductive components such as motors and coiled cables.

How to perform low current continuity measurement

Step 1 Select the **Continuity** function with the function selector switch and select the **Cont** mode with the ▲▼ and ◄►navigation keys. The following menu will be displayed:

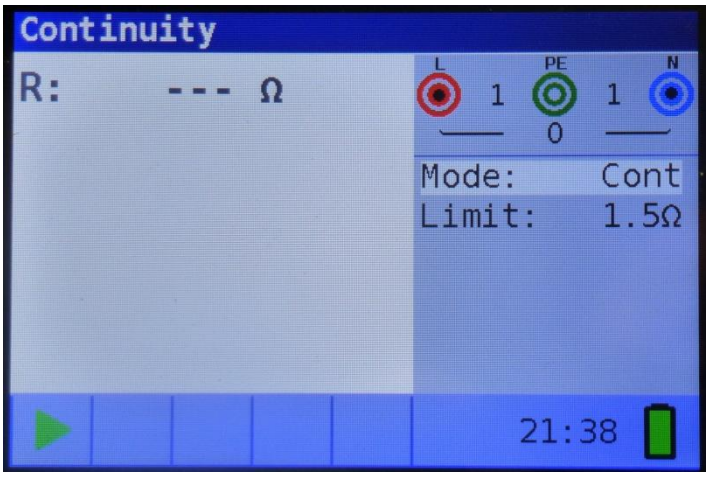

Figure 5-8: Continuity measurement menu

Step 2 Set the following limit value:

- **Limit:** limit resistance value using the ▲▼ and ◄►navigation keys.

Step 3 Connect test cable to the instrument and the item under test. Follow the connection diagram shown in figures 5.10 and 5.11 to perform the **Continuity** measurement.

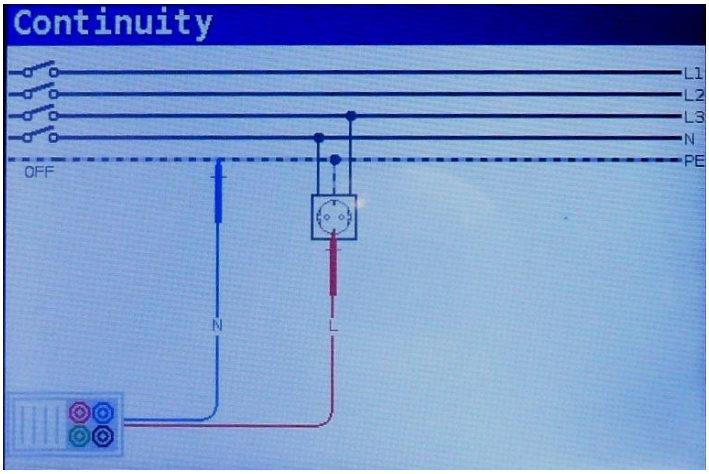

Figure 5-9: Connection of universal test cable

Step 4 Check the warnings and online voltage/terminal monitor on the display before starting the measurement. If everything is OK and the ⌒ is shown, press the TEST key to start the measurement. The actual measuring result with ✎ or ✖ indication (if applicable) will be displayed during the measurement.
As this is a continuous test, the function will require stopping. To stop the measurement at any time press the TEST key again. The last measured result will be displayed together with the ✎ or ✖ indication (if applicable).

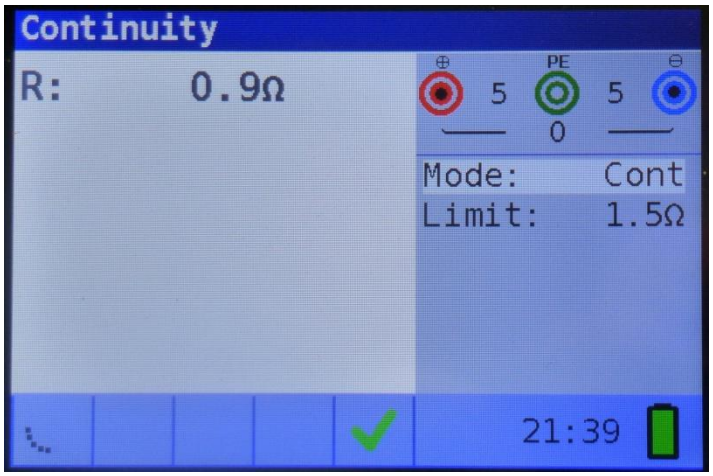

Figure 5-10: Example of Low current continuity measurement result

Displayed result:

R ..... Low current continuity resistance result.

I ..... Current used in the measurement

Warning:

- Low current continuity measurement should only be performed on de-energized objects!

Notes:

- If a voltage of higher than 10 V exists between test terminals, the continuity measurement will not be performed.
  Before performing a continuity measurement, compensate for the test lead resistance (if necessary).

5.3 Testing RCDs

When testing RCDs, the following sub-functions can be performed:

- Contact voltage measurement,
- Trip-out time measurement,
- Trip-out current measurement,
- RCD autotest.

In general, the following parameters and limits can be set when testing RCDs:

- Limit contact voltage,
- Nominal differential RCD trip-out current,
- Multiplier of nominal differential RCD trip-out current,
- RCD type,
- Test current starting polarity.

For possible parameters that could be set look into specification tables at the end of this manual.

5.3.1 Limit contact voltage

Safety contact voltage is limited to 50 V_{AC} for standard domestic area. In special environments (hospitals, wet places, etc.) contact voltages up to 25 V_{AC} are permitted. Limit contact voltage can be set in contact voltage **Uc** function only!

5.3.2 Nominal differential trip-out current

Nominal differential current is the rated trip-out current of an RCD. The following RCD current ratings can be set: 6 mA (*), 10 mA, 30 mA, 100 mA, 300 mA, 500 mA , 650 mA (*) and 1000 mA (*). (* optional)

5.3.3 Multiplier of nominal residual current

Selected nominal differential current can be multiplied by ½, 1, 2 or 5.

5.3.4 RCD type and test current starting polarity

The PCE-ITE 55 SERIESinstrument enables testing of general (non-delayed) and selective (time-
delayed) RCDs. The types of RCD the instrument is suitable for testing include:

- Alternating residual current (AC type),
- Pulsating DC residual current (A type).
- pure or nearly pure DC residual current (B type) (depends on model).
- special RCDs for EVSE applications.

Test current starting polarity can be started with the positive half-wave at 0^0 or with the negative half-wave at 180^0.

positive start polarity (0°) *negative start polarity (180°)*

Figure 5-11: Test current started with the positive or negative half-wave

S

5.3.5 Testing selective (time-delayed) RCDs

Selective RCDs demonstrate delayed response characteristics. Trip-out performance is influenced due to pre-loading during measurement of contact voltage. In order to eliminate the pre-loading a time delay of 30 s is inserted before performing the trip-out test.

5.3.6 Contact voltage

Leakage current flowing to the PE terminal causes a voltage drop across earth resistance, which is called contact voltage (Uc). This voltage is present on all accessible parts connected to the PE terminal and should be lower than the safety limit voltage.
The parameter contact voltage is measured without tripping-out the RCD. R_L is a fault loop resistance and is calculated as follows:

$$R_L = \frac{U_C}{I_{\Delta N}}$$

Displayed contact voltage relates to the rated nominal differential current of the RCD and is multiplied by a safety factor. See the table 5.1 for detailed contact voltage calculation.

RCD type	Contact voltage Uc
G G	Uc ∝ 1.05×$I_{\Delta N}$
S S	Uc ∝ 1.05×2×$I_{\Delta N}$
G G	Uc ∝ 1.05×$\sqrt{2}$ ×$I_{\Delta N}$
S S	Uc ∝ 1.05×2×$\sqrt{2}$ ×$I_{\Delta N}$

Table 5-1*: Relationship between Uc and $I_{\Delta N}$*

How to perform contact voltage measurement

Step 1 Select the **RCD** function with the function selector switch and select the **Uc** mode with the ▲▼ and ◀▶navigation keys. The following menu will be displayed:

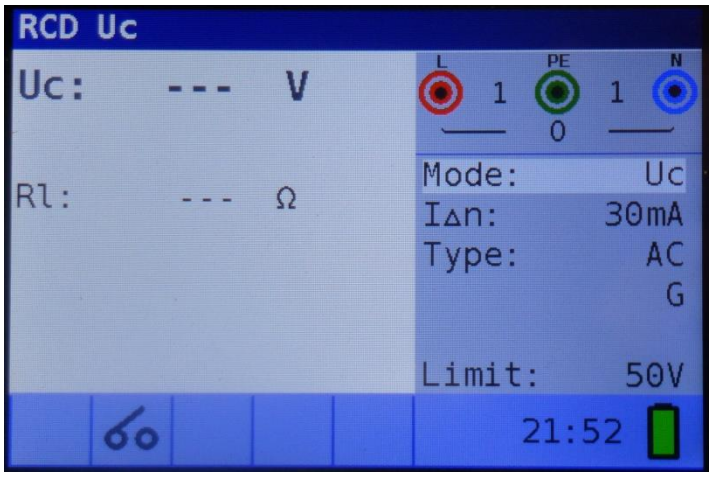

Figure 5-12: Contact voltage measurement menu

Step 2 Set the following measuring parameters and limit values:

- $I_{\Delta N}$: Nominal residual current,
- **Type**: RCD type,
- **Limit:** Limit contact voltage.

Step 3 Connect the test leads to the instrument and follow the connection diagram shown in figure 5.15 to perform contact voltage measurement.

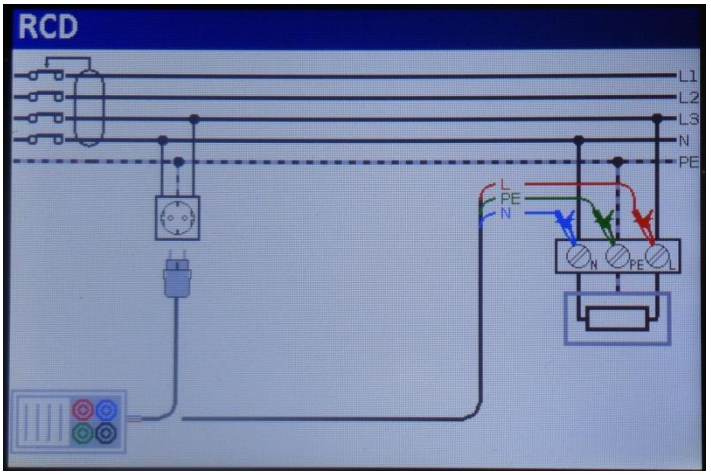

Figure 5-13: Connection of plug test cable or universal test cable

Step 4 Check for any warnings and check the online voltage/terminal monitor on the display before starting the measurement. If everything is ok and the ▶ is shown, press the TEST key. After performing the measurement, the results appear on the display together with the ✎ or ✖ I indication.

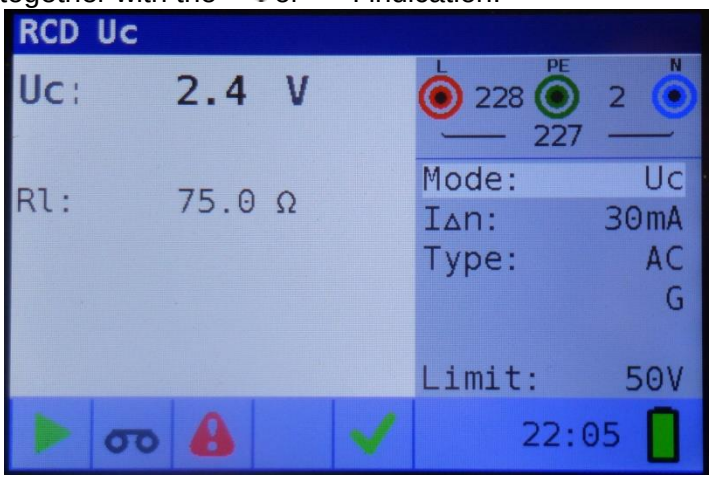

Figure 5-14: Example of contact voltage measurement results

Displayed results:
Uc ..... Contact voltage.
Rl ..... Fault loop resistance.
Limit ..... Limit earth fault loop resistance value according to BS 7671.

Notes:

- Parameters set in this function are also kept for all other RCD functions!
- The measurement of contact voltage does not normally trip an RCD. However, the trip limit may be exceeded as a result of leakage currents flowing through the PE protective conductor or a capacitive connection between the L and PE conductor.
- RCD trip-lock sub-function (function selected to **LOOP RCD** option) takes longer to complete but offers much better accuracy of a fault loop resistance result (in

comparison with the R_L sub-result in **Contact voltage** function).

5.3.7 Trip-out time

Trip-out time measurement is used to verify the effectiveness of an RCD. This is achieved by a test simulating an appropriate fault condition. Trip-out times vary between standards and are listed below.

Trip-out times according to BS EN 61008 / BS EN 61009:

	½×$I_{\Delta N}$ *)	$I_{\Delta N}$	2×$I_{\Delta N}$	5×$I_{\Delta N}$
General (non-delayed) RCDs	t_Δ > 300 ms	t_Δ < 300 ms	t_Δ < 150 ms	t_Δ < 40 ms
Selective (time-delayed) RCDs	t_Δ > 500 ms	130 ms < t_Δ < 500 ms	60 ms < t_Δ < 200 ms	50 ms < t_Δ < 150 ms

Trip-out times according to BS 7671:

	½×$I_{\Delta N}$ *)	$I_{\Delta N}$	2×$I_{\Delta N}$	5×$I_{\Delta N}$
General (non-delayed) RCDs	t_Δ > 1999 ms	t_Δ < 300 ms	t_Δ < 150 ms	t_Δ < 40 ms
Selective (time-delayed) RCDs	t_Δ > 1999 ms	130 ms < t_Δ < 500 ms	60 ms < t_Δ < 200 ms	50 ms < t_Δ < 150 ms

*) Test current of ½×$I_{\Delta N}$ cannot cause trip-out of the RCDs.

Trip-out times according to IEC 62955:

	I_ΔNdc	10×I_ΔNdc	33×I_ΔNdc	
6 mADC RCDs	t_Δ < 10.000 ms	t_Δ < 300 ms	t_Δ < 100 ms	
	I_ΔN	2×I_ΔN	5×I_ΔN	167×I_ΔN
30 mAAC RCDs	no trip	t_Δ < 300 ms	t_Δ < 80 ms	t_Δ < 80 ms

How to perform trip-out time measurement

Step 1 Select the **RCD** function with the function selector switch and select the **Time** mode with the ▲▼ and ◀▶navigation keys. The following menu will be displayed:

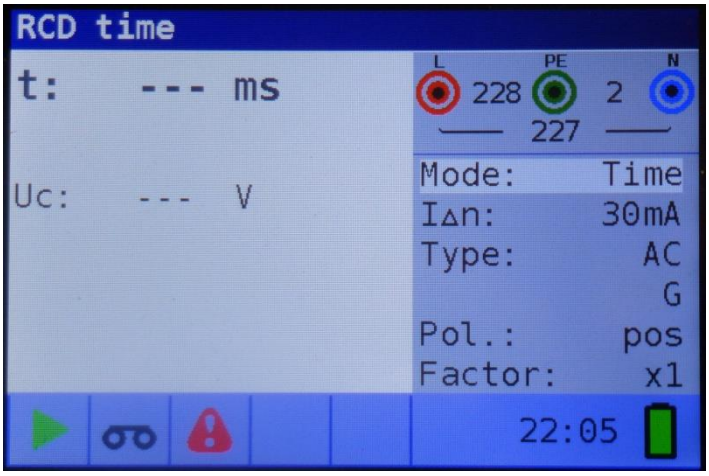

Figure 5-15: Trip-out time measurement menu

Step 2 Set the following measuring parameters:

- **$I_{\Delta N}$**: Nominal differential trip-out current,
- **Factor:** Nominal differential trip-out current multiplier,

- **Type:** RCD type and
- **Pol.:** Test current starting polarity.

Step 3 Connect the leads to the instrument and follow the connection diagram shown in figure 5.15 (see the chapter *5.3.6 Contact voltage*) to perform trip-out time measurement.

Step 4 Check for any warnings and check the online voltage/terminal monitor on the display before starting the measurement. If everything is ok and the ↄ is shown, press the TEST key. After performing the measurement, the results appear on the display together with the ✎ or ✖ indication.

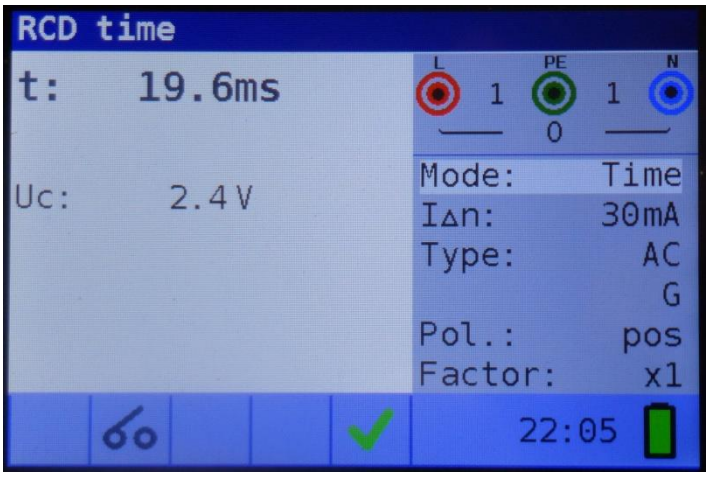

Figure 5-16: Example of trip-out time measurement results

Displayed results:

t.....Trip-out time,
U_C.....Contact voltage.

Notes:

- Parameters set in this function are also transferred onto all other RCD functions!
- RCD trip-out time measurement will be performed only if the contact voltage at nominal differential current is lower than the limit set in the contact voltage setting!
- The measurement of the contact voltage in pre-test does not normally trip an RCD. However, the trip limit may be exceeded as a result of leakage current flowing through the PE protective conductor or a capacitive connection between L and PE conductors.

5.3.8 Trip-out current

This test is used to determine the minimum current required to trip the RCD. After the measurement has been started, the test current generated by the instrument is continuously increased, starting at $0.2\times I_{\Delta N}$ to $1.1\times I_{\Delta N}$ (to $1.5\times I_{\Delta N}$ / $2.2\times I_{\Delta N}$ ($I_{\Delta N}$ =10 mA) for pulsating DC residual currents), until the RCD trips.

How to perform trip-out current measurement

Step 1 Select the **RCD** function with the function selector switch and select the **Ramp** mode with the ▲▼ and ◀▶ navigation keys. The following menu will be displayed:

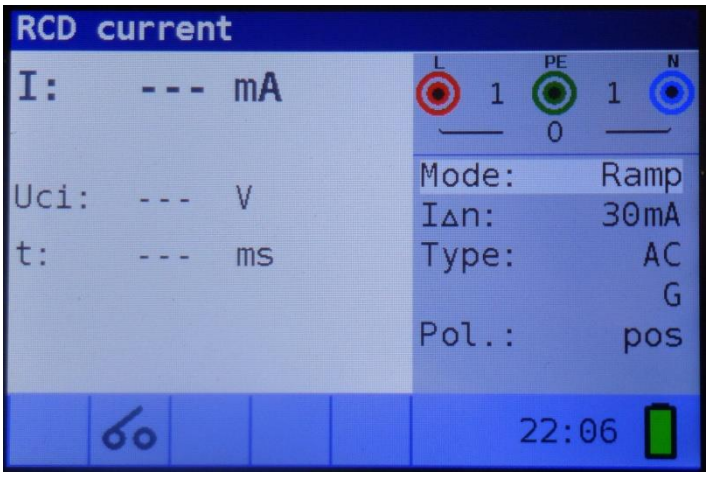

Figure 5-17: Trip-out current measurement menu

Step 2 By using cursor keys the following parameters can be set in this measurement:

- $I_{\Delta N}$: Nominal residual current,
- **Type:** RCD type,
- **Pol.:** Test current starting polarity.

Step 3 Connect the test leads to the instrument and follow the connection diagram shown in figure 5.15 (see the chapter *5.3.6 Contact voltage*) to perform trip- out current measurements.

Step 4 Check for any warnings and check the online voltage/terminal monitor on the display before starting the measurement. If everything is ok and the is shown, press the TEST key. After performing the measurement, the results appear on the display together with the or indication.

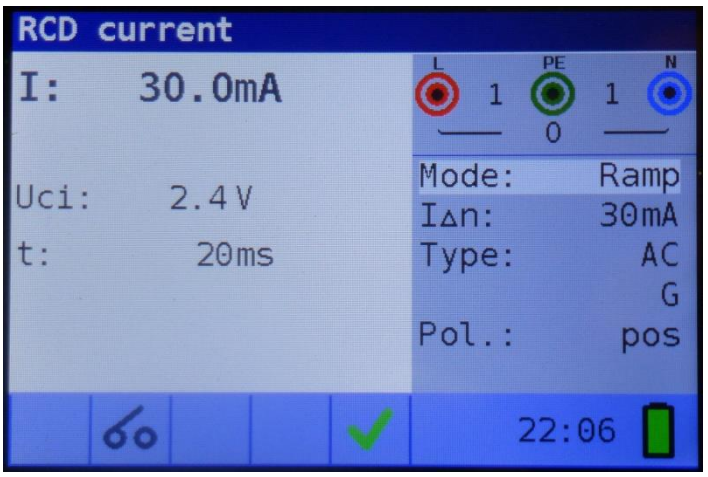

Figure 5-18: Example of trip-out current measurement result

Displayed results:

I…….. Trip-out current,
Uci ..... Contact voltage,
t..... Trip-out time.

Notes:

- Parameters set in this function are also kept for other RCD functions!
- RCD trip-out current measurement will be performed only if the contact voltage at nominal differential current is lower than set limit contact voltage!
- The measurement of contact voltage in the pre-test does not normally trip an RCD. However, the trip limit may be exceeded as a result of leakage current flowing through the PE protective conductor or a capacitive connection between L and PE conductors.

5.3.9 Autotest

The purpose of the autotest function is to perform a complete RCD testing and measurement of most important associated parameters (contact voltage, fault loop resistance and trip-out time at different fault currents) with one press of a button. If a faulty parameter is noticed during the autotest, the test will stop to highlight the need for further investigation.

Notes:

- The measurement of contact voltage in the pre-test does not normally trip an RCD. However, the trip limit may be exceeded as a result of leakage current flowing through the PE protective conductor or a capacitive connection between L and PE conductors.
- The autotest sequence stops when the trip-out time is out of allowed time period.

5.3.9.1 How to perform RCD autotest

Step 1 Select the **RCD** function with the function selector switch and select the **Auto** mode with the ▲▼ and ◀▶navigation keys. The following menu will be displayed:

Figure 5-19: RCD autotest menu

Step 2 Set the following measuring parameters:

- $I_{\Delta N}$: Nominal differential trip-out current,
- **Type:** RCD type.

Step 3 Connect the test leads to the instrument and follow the connection diagram shown in figure 5.15 (also see the chapter *5.3.6 Contact voltage*) to perform the RCD autotest.

Step 4 Check for any warnings and check the online voltage/terminal monit on the display before starting the measurement. If everything is ok and the is shown, press the TEST key. The autotest sequence will then start to run as follows:

1. Trip-out time measurement with the following measurement parameters:
   - Test current of $I_{\Delta N}$,
   - Test current started with the positive half-wave at 0°.

Measurement normally trips an RCD within allowed time period. The following menu is displayed:

Figure 5-20: Step 1 RCD autotest results

After re-activating the RCD, the autotest sequence automatically proceeds with step 2.

2. Trip-out time measurement with the following measurement parameters:
   - Test current of $I_{\Delta N}$,
   - Test current started with the negative half-wave at 180°.

Measurement normally trips an RCD. The following menu is displayed:

Figure 5-21: Step 2 RCD autotest results

After re-activating the RCD, the autotest sequence automatically proceeds with step 3.

3. Trip-out time measurement with the following measurement parameters:

- Test current of 5× $I_{\Delta N}$,
- Test current started with the positive half-wave at 0^0.

Measurement normally trips an RCD within allowed time period. The following menu is displayed:

Figure 5-22: Step 3 RCD autotest results

After re-activating the RCD the autotest sequence automatically proceeds with step 4.

4. Trip-out time measurement with the following measurement parameters:

- Test current of 5× $I_{\Delta N}$,
- Test current started with the negative half-wave at 180^0.

Measurement normally trips an RCD within allowed time period. The following menu is displayed:

Figure 5-23: Step 4 RCD autotest results

After re-activating the RCD the autotest sequence automatically proceeds with step 5.

5. Trip-out time measurement with the following measurement parameters:

- Test current of ½× $I_{\Delta N}$,
- Test current started with the positive half-wave at 0^0.

Measurement does not normally trip an RCD. The following menu is displayed:

Figure 5-24: Step 5 RCD autotest results

After performing step 5 the RCD autotest sequence automatically proceeds with step 6.

6. Trip-out time measurement with the following measurement parameters:

- Test current of ½× $I_{\Delta N}$,
- Test current started with the negative half-wave at 180^0.

Measurement does not normally trip an RCD. The following menu is displayed:

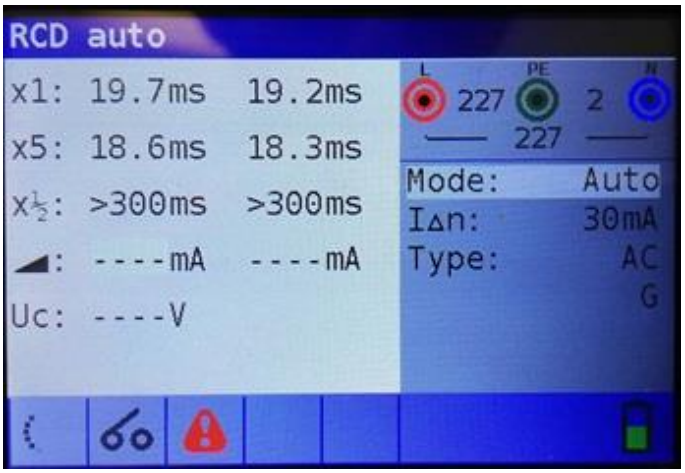

Figure 5-25: Step 6 RCD autotest results

7. Ramp test measurement with the following measurement parameters:

- Test current started with the positive half-wave at 0^0.

This measurement determine the minimum current required to trip the RCD. After the measurement has been started, the test current generated by the instrument is continuously increased, until the RCD trips. The following menu is displayed:

Figure 5-26: Step 7 RCD autotest results

8. Ramp test measurement with the following measurement parameters:

- Test current started with the negative half-wave at 180^0.

This measurement determine the minimum current required to trip the RCD. After the measurement has been started, the test current generated by the instrument is continuously increased, until the RCD trips. The following menu is displayed:

Figure 5-27: Step 8 RCD autotest results

Displayed results:
x1 (left).....Step 1 trip-out time result, t3 ($I_{\Delta N}$, 0^0),
x1 (right).....Step 2 trip-out time result, t4 ($I_{\Delta N}$, 180^0),
x5 (left).....Step 3 trip-out time result, t5 (5× $I_{\Delta N}$, 0^0),
x5 (right).....Step 4 trip-out time result, t6 (5× $I_{\Delta N}$, 180^0),
x½ (left).....Step 5 trip-out time result, t1 (½×$I_{\Delta N}$, 0^0),
x½ (right).....Step 6 trip-out time result, t2 (½×$I_{\Delta N}$, 180^0),
IΔ (+)……Step 7 trip-out current ((+) positive polarity)
IΔ (-)…….Step 8 trip-out current ((-) negative polarity)
Uc ..... Contact voltage for rated $I_{\Delta N}$.

Note:

- the **x1** Auto tests will be automatically skipped for RCD type B with rated residual currents of $I_{\Delta N}$ = 1000 mA
- the **x5** Auto tests will be automatically skipped in the following cases:

  RCD type AC with rated residual currents of $I_{\Delta N}$ = 1000 mA

  RCD type A and B with rated residual currents of $I_{\Delta N}$ >= 300 mA
- In these cases, the auto test result passes if the t1 to t4 results pass, and on the display are omitted t5 and t6.

5.3.10 WARNINGS

- Leakage currents in the circuit following the residual current device (RCD) may influence the measurements.
- Special conditions in residual current devices (RCD) of a particular design, for example of type S (selective and resistant to impulse currents) shall be taken into consideration.
- equipment in the circuit following the residual current device (RCD) may cause a considerable extension of the operating time. Examples of such equipment might be connected capacitors or running motors.

5.4 Fault loop impedance and prospective fault current

The loop impedance function has three sub-functions available:

LOOP IMPEDANCE sub-function performs a fast fault loop impedance measurement on supply systems which do not contain RCD protection.
LOOP IMPEDANCE RCD trip-lock sub-function performs fault loop impedance measurement on supply systems which are protected by RCDs
LOOP IMPEDANCE Rs sub-function with configurable RCD-value performs fault loop impedance measurement on supply systems which are protected by RCDs

5.4.1 Fault loop impedance

The fault loop impedance measures the impedance of the fault loop in the event that a short-circuit to an exposed conductive part occurs (i.e. a conductive connection occurs between the phase conductor and protective earth conductor). In order to measure loop impedance, the instrument uses a high-test current.
Prospective fault current (IPFC) is calculated on the basis of the measured resistance as follows:

$$I_{PFC} = \frac{U_N \times scaling\ factor}{Z_{L-PE}}$$

Where:

Nominal input voltage U_N	Voltage range
115V	(93 V ≤ $U_{L\text{-}PE}$ < 134 V)
230V	(185 V ≤ $U_{L\text{-}PE}$ ≤ 266 V)

How to perform fault loop impedance measurement

Step 1 Select the **LOOP** function with the function selector switch and select the **LOOP** mode with the ▲▼ and ◀▶navigation keys. Then select desired **Type** (select various types or custom or off), **Time** and **Curr** option values with the ▲▼ and ◀▶ navigation keys. The following menu is displayed:

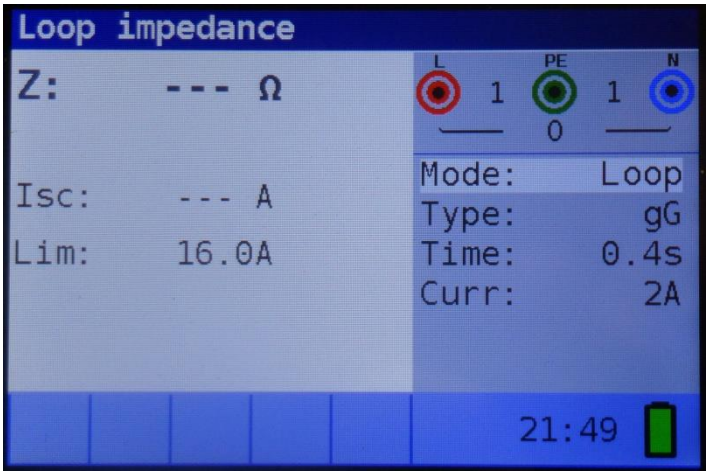

Figure 5-28: Loop impedance measurement menu

Step 2 Connect the test leads to the instrument and follow the connection diagram shown in the figure 5.29 to perform fault loop impedance measurement.

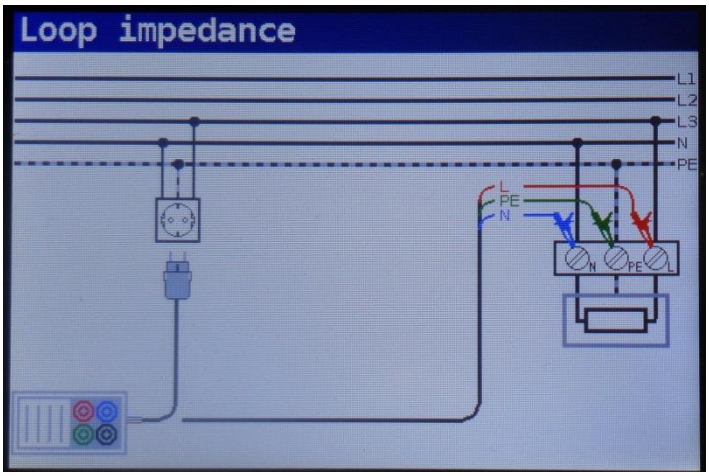

Figure 5-29: Connection of plug cable and universal test cable

Step 3 Check for any warnings displayed on the screen and check the online voltage/terminal monitor before starting the measurement. If everything is ok and the ▶ is shown, press the TEST key. After performing the measurement, the test results will appear on the display.

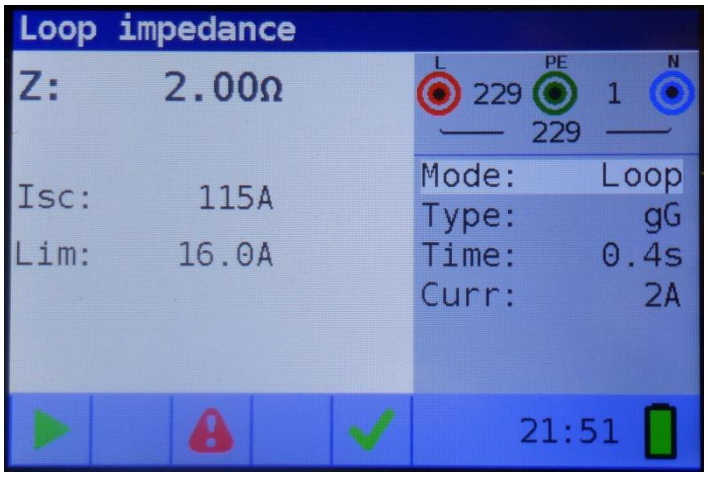

Figure 5-30: Example of loop impedance measurement results

Displayed results:

Z.....Fault loop impedance,
Isc.....Prospective fault current (displayed in amps),

Notes:

- The specified accuracy of test parameters is valid only if mains voltage is stable during the measurement.
- The Fault loop impedance measurement trips RCD protected circuits.

5.4.2 The fault loop impedance test RCD (for RCD protected circuits)

The fault loop impedance is measured with a low test current to avoid tripping the RCD. This function can also be used for fault loop impedance measurement in system equipped with RCDs which have a rated trip-out current of 30 mA and above.

Prospective fault current (IPFC) is calculated on basis of measured resistance as follows:

$$I_{PFC} = \frac{U_N \times scaling\ factor}{Z_{L-PE}}$$

Where:

Nominal input voltage U_N	Voltage range
115V	(93 V ≤ $U_{L\text{-}PE}$ < 134 V)
230V	(185 V ≤ $U_{L\text{-}PE}$ ≤ 266 V)

How to perform RCD trip-lock measurement

Step 1 Select the **LOOP** function with the function selector switch and select the **RCD** mode with the ▲▼ and ◄►navigation keys. Then select desired **Type** (select various types or custom or off), **Time** and **Curr** option values with the ▲▼ and ◄►navigation keys. The following menu is displayed:

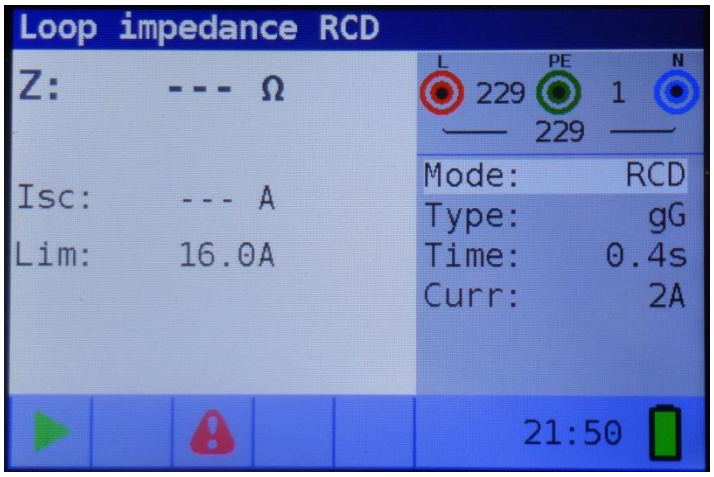

Figure 5-31: Trip-lock function menu

Step 2 Connect the appropriate test leads to the instrument and follow the connection diagram shown in figure 5.13 to perform RCD trip-lock measurement (see chapter *5.3.6 Contact voltage*).

Step 3 Check for warnings on the display and check the online voltage/terminal monitor before starting the measurement. If everything is ok and the ▶ is shown, press the TEST key. After performing the measurement, the results will appear on the display.

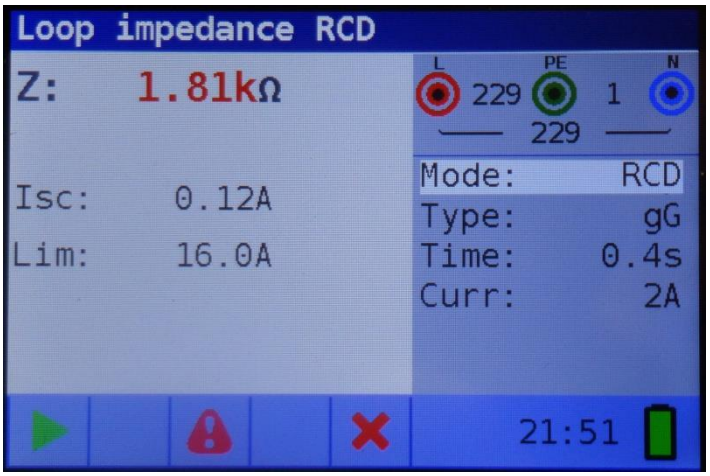

Figure 5-32: Example of fault loop impedance measurement results using RCD function

Displayed result:

Z.....Fault loop impedance,
I_{sc}.....Prospective fault current,

Notes:

- The measurement of fault loop impedance using trip-lock function does not normally trip an RCD. However, if the trip limit may be exceeded as a result of leakage current flowing through the PE protective conductor or a capacitive connection between L and PE conductors.
- The specified accuracy of test parameter is valid only if mains voltage is stable during the measurement.

5.4.3 The fault loop impedance test Rs (for adjustable current)

The fault loop impedance is measured with a low test current to avoid tripping the RCD. It is possible to adjust the value of the RCD, while the test current depends on the chosen value. By this function it is possible to test each RCD-type with the maximum possible current without tripping the RCD.

Prospective fault current (IPFC) is calculated on basis of measured resistance as follows:

$$I_{PFC} = \frac{U_N \times scaling\ factor}{Z_{L-PE}}$$

Where:

Nominal input voltage U_N	Voltage range
115V	(93 V ≤ $U_{L\text{-}PE}$ < 134 V)
230V	(185 V ≤ $U_{L\text{-}PE}$ ≤ 266 V)

How to perform Rs trip-lock measurement

Step 1 Select the **LOOP** function with the function selector switch and select the **Rs** mode with the ▲▼ and ◀▶navigation keys. Then select desired **Type** (select various types or custom or off), **current**, **Limit** and **scaling factor** option values with the ▲▼ and ◀▶navigation keys. The following menu is displayed:

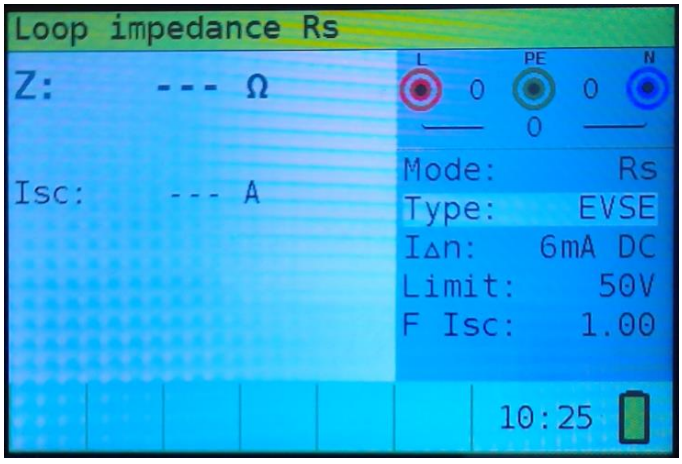

Figure 5-333: Loop impedance Rs function menu

Step 2 Connect the appropriate test leads to the instrument and follow the connection diagram shown in figure 5.13 to perform RCD trip-lock measurement (see chapter *5.3.6 Contact voltage*).

Step 3 Check for warnings on the display and check the online voltage/terminal monitor before starting the measurement. If everything is ok and the ▶ is shown, press the TEST key. After performing the measurement, the results will appear on the display.

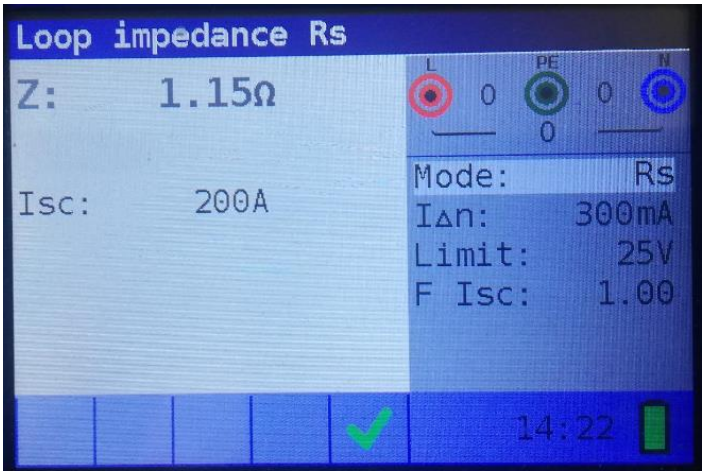

Figure 5-344: Example of fault loop impedance measurement results using Rs function

Displayed result:

Z.....Fault loop impedance,
I_{sc}.....Prospective fault current,

Notes:

- The measurement of fault loop impedance using trip-lock function does not normally trip an RCD. However, if the trip limit may be exceeded as a result of leakage current flowing through the PE protective conductor or a capacitive connection between L and PE conductors.
- The specified accuracy of test parameter is valid only if mains voltage is stable during the measurement.

5.5 Line impedance and prospective short-circuit current

The line impedance is a measurement of the impedance of the current loop when a short-circuit to the neutral conductor occurs (conductive connection between phase conductor and neutral conductor in single-phase system or between two phase conductors in three-phase system). A high test current is used to perform the line impedance measurement.

Prospective short circuit current is calculated as follows:

$$I_{PFC} = \frac{U_N \times scaling\ factor}{Z_{L-N(L)}}$$

Where:

Nominal input voltage U_N	**Voltage range**
115V	(93 V ≤ $U_{L\text{-}PE}$ < 134 V)
230V	(185 V ≤ $U_{L\text{-}PE}$ ≤ 266 V)
400V	(321V ≤ $U_{L\text{-}PE}$ ≤ 485 V)

How to perform line impedance measurement

Step 1 Select the **LINE IMPEDANCE** function with the function selector switch. Then select desired **Type** (select various types or custom or off), **Time** and **Curr** option values with the ▲▼ and ◀▶navigation keys. The following menu is displayed:

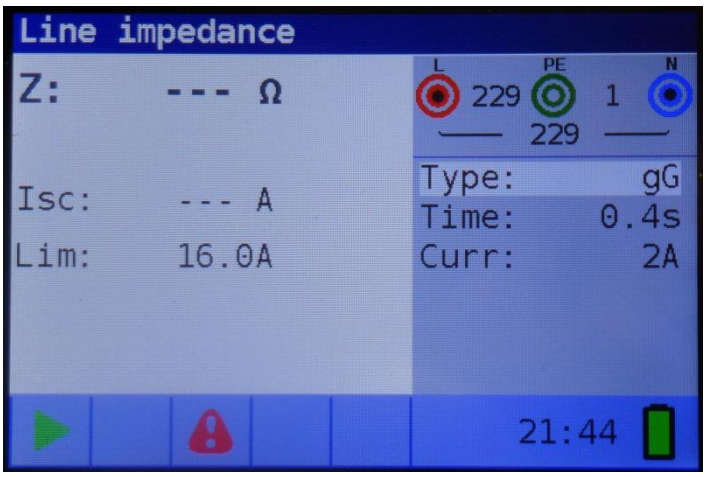

Figure 5-35: Line impedance measurement menu

Step 2 Connect the appropriate test leads to the instrument and follow the connection diagram shown in figure 5.36 to perform phase-neutral or phase- phase line impedance measurement.

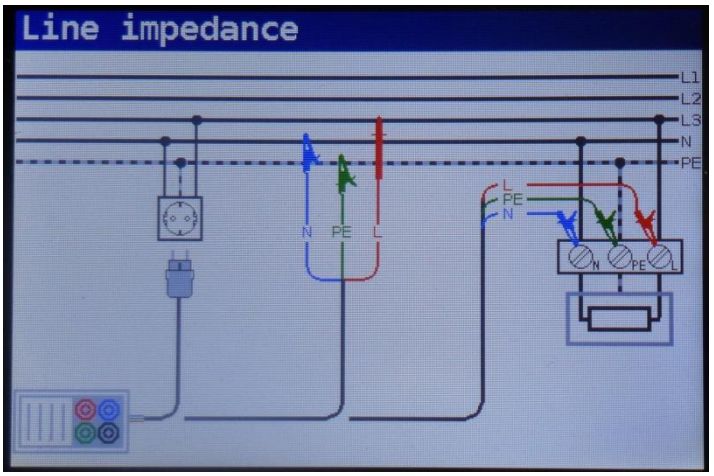

Figure 5-356: Line impedance measurement

Step 3 Check for warnings displayed on the screen and check the online voltage/terminal monitor before starting the measurement. If everything is ok and the ▶ is shown, press the TEST key. After performing the measurement, the results will appear on the display.

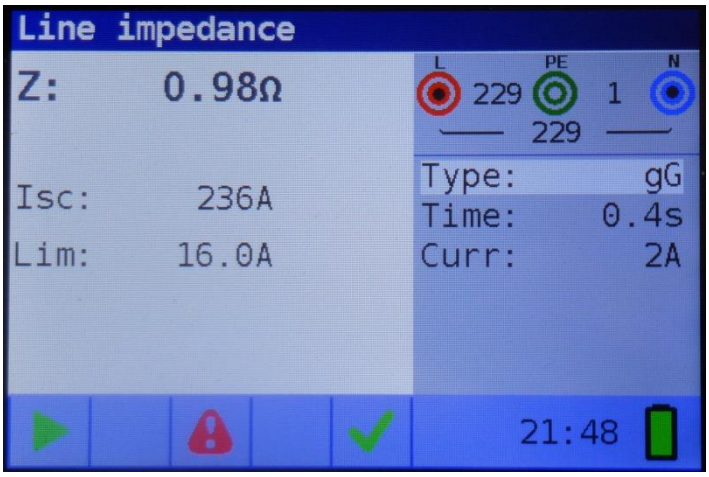

Figure 5-367: Example of line impedance measurement results

Displayed results:

Z.....Line impedance,
I$_{sc}$.....Prospective short-circuit current,

Notes:

- The specified accuracy of the test parameter is valid only if mains voltage is stable during the measurement.

5.5.1 Voltage drop test

The voltage drop function is a measurement of the line impedance (see chapter 5.5) and result is compared to a reference result which has been taken before on some other point of the installation (usually the entry point since this point has the lowest impedance). The voltage drop in %, the impedance and the prospective short circuit current are shown.

The voltage drop in % is calculated as follows:

$$\Delta U = \frac{(Z - Z_{REF}) \times I_N}{U_N}$$

How to perform voltage drop measurement

Step 1 Select the **LINE IMPEDANCE** function with the function selector switch and select Voltage drop with the ▲▼ and ◀▶navigation keys. Then select desired **Type** (select various types or custom or off), **Time** and **Curr** option values with the ▲▼ and ◀▶navigation keys. The following menu is displayed:

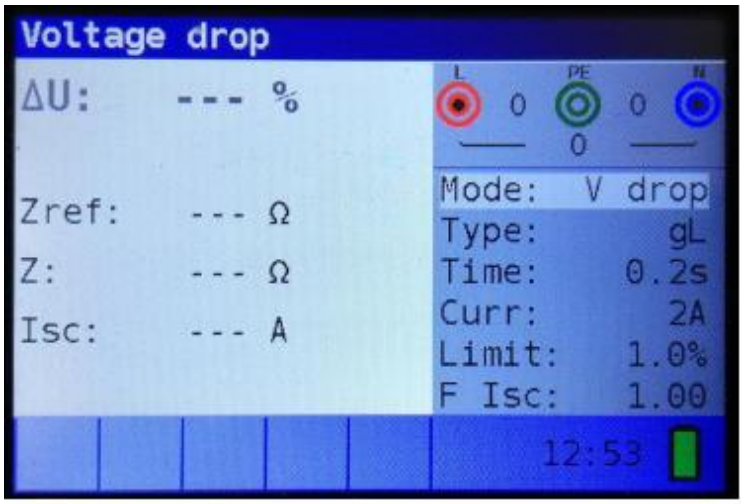

Figure 5-378: Voltage drop measurement menu

Step 2 Connect the appropriate test leads from the reference point to the instrument and follow the connection diagram shown in figure 5.36 to perform phase-neutral or phase- phase line impedance measurement.

Step 3 Press COM key and 'REF' will be shown in display. The device is then ready to take the measurement of the reference position in the installation. Check for warnings displayed on the screen and check the online voltage/terminal monitor before starting the measurement. If everything is ok and the ▶ is shown, press the TEST key. After performing the measurement, the result for Zref will appear on the display.

Step 4 Connect the appropriate test leads from the tested point to the instrument and follow the connection diagram shown in figure 5.36 to perform phase-neutral or phase- phase line impedance measurement. Check for warnings displayed on the screen and check the online voltage/terminal monitor before starting the measurement. If everything is ok and the ▶ is shown, press the TEST key. After performing the measurement, the results will appear on the display.

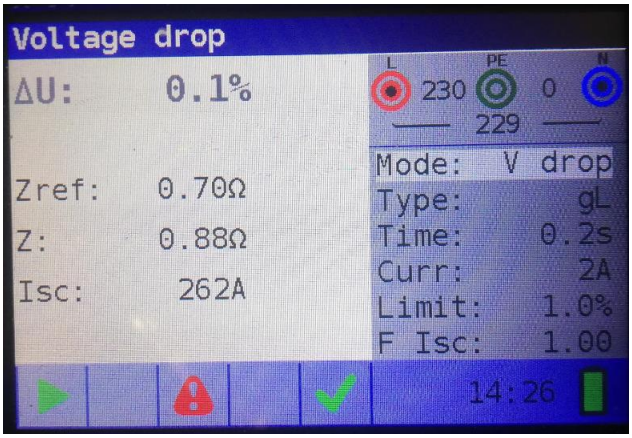

Figure 5-389: Example of voltage drop measurement results

Displayed results:

∆**U……**voltage drop of the test point compared to the reference point

Zref ..... Line impedance of the reference point

Z..... Line impedance of the test point
I_{sc}..... Prospective short-circuit current of the test point

Notes:

- The specified accuracy of the test parameter is valid only if mains voltage is stable during the measurement.

5.6 Phase sequence testing

In practice, we often deal with the connection of three-phase loads (motors and other electro-mechanical machines) to three-phase mains installation. Some loads (ventilators, conveyors, motors, electro-mechanical machines, etc.) require a specific phase rotation and some may even be damaged if the rotation is reversed. This is why it is advisable to test phase rotation before connection is made.

How to test the phase sequence

Step 1 Select the **VOLTAGE** function with the function selector switch. The following menu is displayed:

Figure 5-40: Phase rotation test menu

Step 2 Connect test cable to the PCE-ITE 55 SERIESinstrument and follow the connection diagram shown in figure 5.41 to test phase sequence.

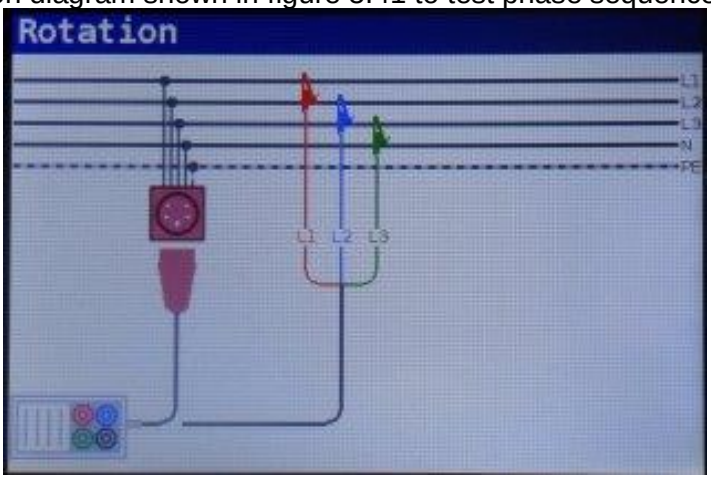

Figure 5-41: Connection of universal test cable and optional three phase cable

Step 3 Check for warnings on the display and check the online voltage/terminal monitor. The phase sequence test is a continuously running test hence the results will be displayed as soon as the full test lead connection to the item under test has been made. All three-phase voltages are displayed in order of their sequence represented by the numbers 1, 2 and 3.

Figure 5-42: Example of phase sequence test result

Displayed results:

Freq……..Frequency,
Rotation ……. Phase sequence,
-.-.-…….Irregular rotation value.

5.7 Voltage and frequency

Voltage measurements should be carried out regularly while dealing with electric installations (carrying out different measurements and tests, looking for fault locations, etc.). Frequency is measured for example when establishing the source of mains voltage (power transformer or individual generator).

How to perform voltage and frequency measurement

Step 1 Select the **VOLTAGE** function with the function selector switch. The following menu is displayed:

Figure 5-43: Voltage and frequency measurement menu

Step 2 Connect test cable to the PCE-ITE 55 SERIESinstrument and follow the connection diagram shown in figure 5.44 to perform a voltage and frequency measurement.

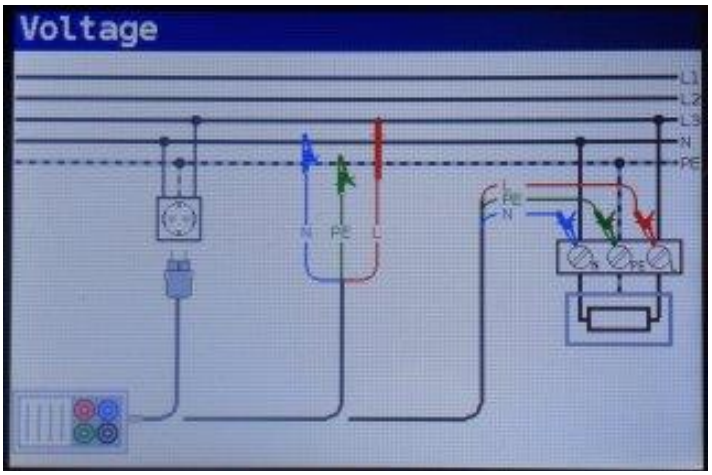

Figure 5-394: Connection diagram

Step 3 Check the displayed warnings. The Voltage and Frequency test continually runs, showing fluctuations as they occur, these results are shown on the display during measurement.

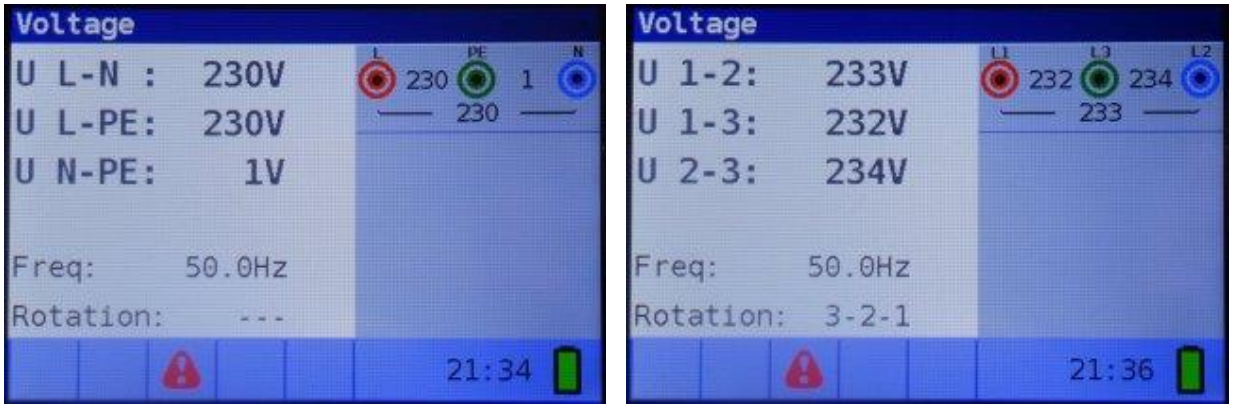

Figure 5-405: Examples of voltage and frequency measurements

Displayed results:

U L-N ..... Voltage between phase and neutral conductors,
U L-PE ..... Voltage between phase and protective conductors,
U N-PE..... Voltage between neutral and protective conductors.

When testing three-phase system the following results are displayed:

U 1-2 ..... Voltage between phases L1 and L2,
U 1-3 ..... Voltage between phases L1 and L3,
U 2-3 ..... Voltage between phases L2 and L3,

5.8 Earth Resistance

5.8.1. Earth Resistance (Re) - 3-wire, 4wire

PCE-ITE 55 SERIESallows resistance to earth measurement using 3-wire and 4wire measuring method.

How to perform Earth Resistance measurement

Step 1 Select the **Earth Resistance** function with the function selector switch and select the **Re** mode with the ▲▼ and ◀▶navigation keys. The following menu will be displayed:

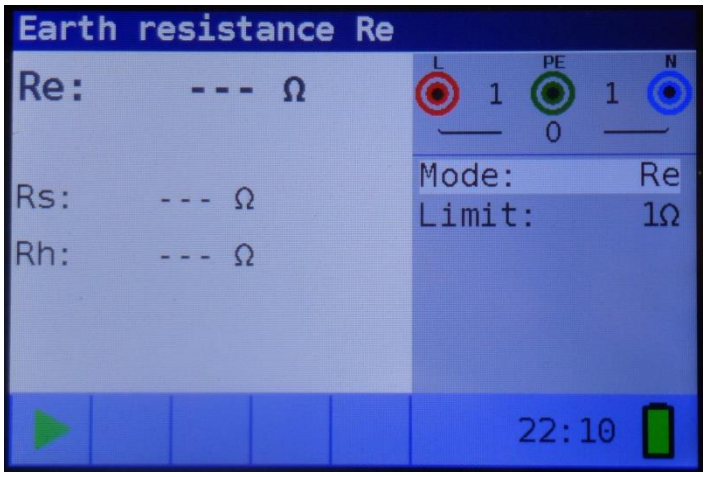

Figure 5-416: Earth Resistance (Re) measurement menu

Step 2 Set the following limit value:

- **Limit:** limit resistance value using the ▲▼ and ◀▶navigation keys.

Step 3 Follow the connection diagram shown in figures 5.47 to perform the **Earth Resistance** measurement with 4 wires.

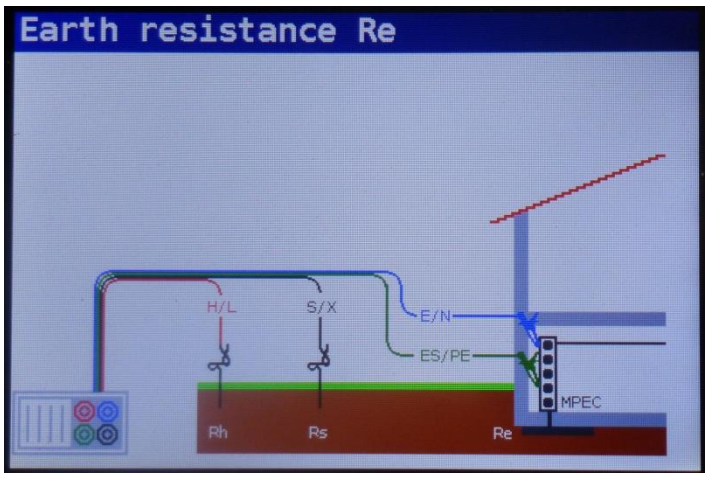

Figure 5-47: 4 wire connection diagram

Follow the connection diagram shown in figures 5.48 to perform the **Earth Resistance** measurement with 3 wires (ES connected to E).

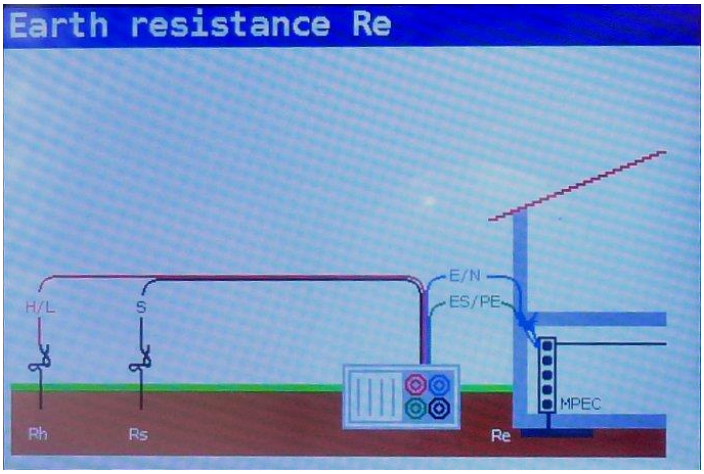

Figure 5-48: 3 wire connection diagram

Step 4 Check for any warnings and the online voltage/terminal monitor on the display before starting the measurement. If everything is ok and the is shown, press the TEST key.
After performing the measurement, the results appear on the display together with the or indication (if applicable).

Figure 5-49: Example of resistance to earth measurement results

Displayed result:
Re……resistance to earth.
Rs…… Resistance of S (potential) probe
Rh…… Resistance of H (current) probe

Notes:

- If a voltage of higher than 10 V exists between test terminals, the Earth Resistance measurement will not be performed.

5.8.2. Specific earth resistance (Ro)

It is advisable to measure Earth Resistivity, when defining parameters of earthing system (required length and surface of earth electrodes, most appropriate depth of installing earthing system etc.) in order to reach more accurate calculations.

How to perform Specific Earth Resistance measurement

Step 1 Select the **Earth Resistance** function with the function selector switch and select the **Ro** mode with the ▲▼ and ◀▶navigation keys. The following menu will be displayed:

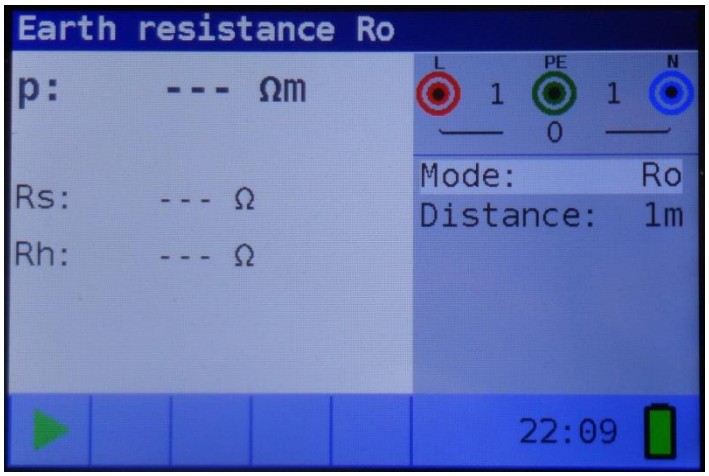

Figure 5-50: Specific Earth Resistance (Ro) measurement menu

Step 2 Set the following limit value:

- **Distance:** set distance "a" between test rods using the ▲▼ and ◀▶navigation keys.

Step 3 Follow the connection diagram shown in figures 5.51 to perform the **Specific Earth Resistance** measurement.

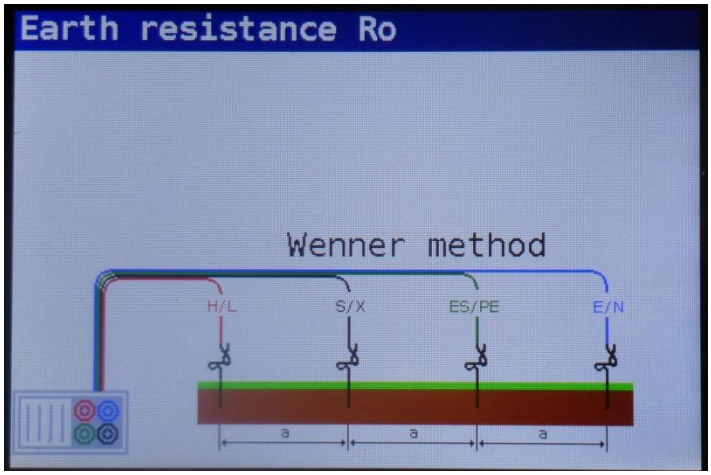

Figure 5-51: Connection diagram

Step 4 Check for any warnings and the online voltage/terminal monitor on the display before starting the measurement. If everything is ok and the ⌒ is shown, press the TEST key.
After performing the measurement, the results appear on the display together with the ✎ or ✖ indication (if applicable).

Figure 5-52: Example of specific earth resistance measurement results

Displayed result:
Ro…… specific earth resistance.
Rs…… Resistance of S (potential) probe
Rh…… Resistance of H (current) probe

Notes:

- If a voltage of higher than 10 V exists between test terminals, the Earth Resistance measurement will not be performed.

6 Maintenance

6.1. Replacing fuses

There are three fuses under back battery cover of the PCE-ITE 55 SERIESinstrument.

- F3

M 0.315 A / 250 V, 20×5 mm
This fuse protects internal circuitry of low-value resistance function if test probes are connected to the mains supply voltage by mistake.

- F1, F2

F 4 A / 500 V, 32×6.3 mm
General input protection fuses for the L/L1 and N/L2 test terminals.

Warnings:

- ⚠ Disconnect any measuring accessory from the instrument and ensure that the instrument is turned off before opening the battery/fuse compartment cover, hazardous voltage can exist inside this compartment!
  - Replace any blown fuses with exactly the same type of fuse. The instrument can be damaged and/or operator's safety impaired if this is not performed!

The Position of fuses can be seen in figure 3.4 in chapter 3.3 Back panel.

6.2. Cleaning

No special maintenance is required for the housing. To clean the surface of the instrument use a soft cloth slightly moistened with soapy water or alcohol. Then leave the instrument to dry totally before use.

Warnings:

- Do not use liquids based on petrol or hydrocarbons!
- Do not spill cleaning liquid over the instrument!

6.3. Periodic calibration

It is essential that the test instrument is regularly calibrated in order for the technical specification listed in this manual to be guaranteed. We recommend an annual calibration. The calibration should be done by an authorized technical person only. Please contact your dealer for further information.

6.4. Service

For repairs under warranty, or at any other time, please contact your distributor. Unauthorized person(s) are not allowed to open the PCE-ITE 55 SERIESinstrument. There are no user replaceable components inside the instrument, except for the three fuses inside the battery compartment, refer to chapter *6.1 Replacing fuses*.

6.5. Batteries

- Prevent Memory Effect
  Discharge and recharge the nickel-metal hydride battery's full once in a while. This helps to keep the battery healthy by avoiding crystal development in discharged areas.

- Exercise the Battery
  Do not leave the battery unused for a longer period. This allows crystals to develop, which reduces the battery's ability to hold a charge. A new battery break procedure should be applied to a dormant battery to regain its ability to work properly.

- New Battery Break-in
  New batteries must be fully charged before use since they are bought in discharged conditions. It is essential to charge and discharge the battery completely so that it can regain its maximum rated capacity.

7 Technical specifications

7.1 Insulation resistance

Insulation resistance (nominal voltages 50V_{DC})
Measurement range according to 61557 from 50kΩ-80MΩ

Measuring range (MΩ)	**Resolution (MΩ)**	**Accuracy**
0.1 ÷ 80.0	(0.100 ... 1.999) 0.001 (2.00 ... 80.00) 0.01	±(5 % of reading + 3 digits)

Insulation resistance (nominal voltages 100 V_{DC} and 250 V_{DC})
Measurement range according to 61557 from 100kΩ-199.9MΩ

Measuring range (MΩ)	**Resolution (MΩ)**	**Accuracy**
0.1 ÷ 199.9	(0.100 ... 1.999) 0.001 (2.00 ... 99.99) 0.01 (100.0 ... 199.9) 0.1	±(5 % of reading + 3 digits)

Insulation resistance (nominal voltages 500 V_{DC} and 1000 V_{DC})
Measurement range according to 61557 from 500kΩ-199.9MΩ

Measuring range (MΩ)	**Resolution (MΩ)**	**Accuracy**
0.1 ÷ 199.9	(0.100 ... 1.999) 0.001 (2.00 ... 99.99) 0.01 (100.0 ... 199.9) 0.1	±(2 % of reading + 3 digits)
200 ÷ 999	(200 ... 999) 1	±(10 % of reading)

Voltage

Measuring range (V)	**Resolution (V)**	**Accuracy**
0 ÷ 1200	1	±(3 % of reading + 3 digits)

Nominal voltages..... 50V_{DC}, 100 V_{DC}, 250 V_{DC}, 500 V_{DC}, 1000 V_{DC}
Open circuit voltage..... .. -0 % / +20 % of nominal voltage
Measuring current ..... min. 1 mA at $R_N=U_N \times 1$ kΩ/V
Short circuit current ..... max. 15 mA
The number of possible tests
with a new set of batteries ..... up to 1000 (with 2300mAh battery cells)
Auto discharge after test.

In case the instrument gets moistened the results could be impaired. In such case it is recommended to dry the instrument and accessories for at least 24 hours.

7.2 Continuity resistance

7.2.1 Low R (depends on model)

Measuring range according to EN61557-4 is 0.1 Ω ÷ 1999 Ω.

Measuring range (Ω)	**Resolution (Ω)**	**Accuracy**
0.1 ÷ 20.0	(0.10 Ω ... 19.99 Ω) 0.01 Ω	±(3 % of reading + 3 digits)
20.0 ÷ 1999	(20.0 Ω ... 99.9 Ω) 0.1 Ω (100 Ω ... 1999 Ω) 1 Ω	±(5% of reading)

Open-circuit voltage ..... 5 V_{DC}
Measuring current ..... min. 200 mA into load resistance of 2 Ω
Test lead compensation .....up to 5 Ω
The number of possible tests
with a new set of batteries..... up to 1400 (with 2300mAh battery cells)
Automatic polarity reversal of the test voltage.

7.2.2 Low current continuity

Measuring range (Ω)	**Resolution (Ω)**	**Accuracy**
0.1 ÷ 1999	(0.1 Ω ... 99.9 Ω) 0.1 Ω (100.0 Ω ... 1999 Ω) 1 Ω	±(5 % of reading + 3 digits)

Open-circuit voltage ..... 5 V_{DC}
Short-circuit current ..... max. 7 mA
Test lead compensation ..... up to 5 Ω

7.3 RCD testing

7.3.1 General data

Nominal residual current ……. 6mA (*), 10 mA, 30 mA, 100 mA, 300 mA, 500 mA, 650mA (*), 1000 mA (*)
Nominal residual current accuracy.... -0 / +0.1·$I_Δ$; $I_Δ = I_{ΔN}$, 2×$I_{ΔN}$, 5×$I_{ΔN}$
-0.1·$I_Δ$ / +0; $I_Δ$ = ½×$I_{ΔN}$
Test current shape ..... Sine-wave (AC), DC (B), pulsed (A) (*)
RCD type..... general (G, non-delayed), selective (S, time-delayed), EVSE (*)
Test current starting polarity..... 0^0 or 180^0
Voltage range..... 93V-134V; 185V-266V; 45Hz-65Hz
(*) depends on model

RCD test current selection (r.m.s. value calculated to 20 ms) according to IEC 61009:

	½x$I_{ΔN}$			1x$I_{ΔN}$			2x$I_{ΔN}$			5x$I_{ΔN}$			RCD IΔ		
$I_{ΔN}$ (mA)	AC	A	B	AC	A	B	AC	A	B	AC	A	B	AC	A	B
6 (*)	3	2,1	3	6	12	12	12	24	24	30	60	60	✓	✓	✓
10	5	3,5	5	10	20	20	20	40	40	50	100	100	✓	✓	✓
30	15	10,5	15	30	42	60	60	84	120	150	212	300	✓	✓	✓
100	50	35	50	100	141	200	200	282	400	500	707	1000	✓	✓	✓
300	150	105	150	300	424	600	600	848	na	1500	na	na	✓	✓	✓
500	250	175	250	500	707	1000	1000	1410	na	2500	na	na	✓	✓	✓
650 (*)	325	228	325	650	919	1300	1300	na	na	na	na	na	✓	✓	✓
1000 (*)	500	350	500	1000	1410	na	2000	na	na	na	na	na	✓	✓	✓

(na) not available / (*) depends on model)

7.3.2 Contact voltage

Measuring range according to EN61557-6 is 3.0 V ÷ 49.0 V f. limit contact voltage 25 V.
Measuring range according to EN61557-6 is 3.0 V ÷ 99.0 V for limit contact voltage 50 V.

Measuring range (V)	**Resolution (V)**	**Accuracy**
3.0 ÷ 9.9	0.1	(-0%/+10%) of reading + 5 digits
10.0÷ 99.9	0.1	(-0%/+10%) of reading + 5 digits

Test current ..... max. $0.5\times I_{\Delta N}$
Limit contact voltage..... 25 V, 50 V

Fault loop resistance at contact voltage is calculated as $R_L = \frac{U_C}{I_{\Delta N}}$.

7.3.3 Trip-out time

Complete measurement range corresponds to EN61557-6 requirements. Specified accuracies are valid for complete operating range.

Measuring range (ms)	**Resolution (ms)**	**Accuracy**
0.0 ÷ 500.0	0.1	±3 ms

Test current ..... $½\times I_{\Delta N}$, $I_{\Delta N}$, $2\times I_{\Delta N}$, $5\times I_{\Delta N}$
Multipliers not available see test current selection table

7.3.4 Trip-out current

Measurement range corresponds to EN61557-6 for $I_{\Delta}N \geq 10$mA. Specified accuracies are valid for complete operating range.

Measuring range I_{Δ}	**Resolution I_{Δ}**	**Accuracy**
$0.2\times I_{\Delta N}$ ÷ $1.1\times I_{\Delta N}$ (AC type)	$0.05\times I_{\Delta N}$	$\pm 0.1\times I_{\Delta N}$
$0.2\times I_{\Delta N}$ ÷ $1.5\times I_{\Delta N}$ (A type, $I_{\Delta N}\geq 30$ mA)	$0.05\times I_{\Delta N}$	$\pm 0.1\times I_{\Delta N}$
$0.2\times I_{\Delta N}$ ÷ $2.2\times I_{\Delta N}$ (A type,$I_{\Delta N}$=10 mA)	$0.05\times I_{\Delta N}$	$\pm 0.1\times I_{\Delta N}$
$0.2\times I_{\Delta N}$ ÷ $2.2\times I_{\Delta N}$ (B type)	$0.05\times I_{\Delta N}$	$\pm 0.1\times I_{\Delta N}$

Trip-out time

Measuring range (ms)	**Resolution (ms)**	**Accuracy**
0 ÷ 300	1	±3 **ms**

Contact voltage

Measuring range (V)	**Resolution (V)**	**Accuracy**
3.0 ÷ 9.9	0.1	(-0%/+10%) of reading + 5 digits
10.0 ÷ 99.9	0.1	(-0%/+10%) of reading + 5 digits

7.4 Fault loop impedance and prospective fault current

Zloop L-PE, I_{pfc} sub-function

Measuring range according to EN61557-3 is 0.25 Ω ÷ 1999 Ω.

Measuring range (Ω)	Resolution (Ω) (*)	Accuracy
0.2 ÷ 9999	(0.20 ... 19.99) 0.01 (20.0 ... 99.9)0.1 (100 ... 9999)1	±(5 % of reading + 5 digits)

(*) depends on model

Prospective fault current (calculated value)

Measuring range (A)	Resolution (A)	Accuracy
0.00 ÷ 19.99	0.01	Consider accuracy of fault loop resistance measurement
20.0 ÷ 99.9	0.1	
100 ÷ 999	1	
1.00k ÷ 9.99k	10	
10.0 ÷ 100.0k	100	

Test current (at 230 V)..... 3.4 A, 50Hz Sine wave (10 ms ≤ t_{LOAD} ≤ 15 ms)
Nominal voltage range..... 93 V ÷ 134 V; 185 V ÷ 266 V (45 Hz ÷ 65 Hz)

Zloop L-PE RCD and Rs, I_{pfc}, non trip subfunction

Measuring range according to EN61557 is 0.75 Ω ÷ 1999 Ω.

Measuring range (Ω)	Resolution (Ω) (*)	Accuracy *)
0.4 ÷ 19.99	(0.40 ... 19.99) 0.01	±(5 % of reading + 10 digits)
20.0 ÷ 9999	(20.0 ... 99.9) 0.1 (100 ... 9999) 1	± 10 % of reading

(*) depends on model
*) Acccuracy may be impaired in case of heavy noise on mains voltage.

Prospective fault current (calculated value)

Measuring range (A)	Resolution (A)	Accuracy
0.00 ÷ 19.99	0.01	Consider accuracy of fault loop resistance measurement
20.0 ÷ 99.9	0.1	
100 ÷ 999	1	
1.00k ÷ 9.99k	10	
10.0 ÷ 100.0k	100	

No trip out of RCD.

Nominal voltage range..... 93 V ÷ 134 V; 185 V ÷ 266 V (45 Hz ÷ 65 Hz)

7.5 Line impedance and prospective short-circuit current

Line impedance

Measuring range according to EN61557-3 is 0.25Ω ÷ 1999Ω.

Zline L-L, L-N, $I_{psc\ subfunction}$

Measuring range (Ω)	**Resolution (Ω) (*)**	**Accuracy**
0.2 ÷ 9999	(0.20 ... 19.99) 0.01 (20.0 ... 99.9)0.1 (100 ... 9999)1	±(5 % of reading + 5 digits)

(*) depends on model

Prospective short-circuit current (calculated value)

Measuring range (A)	**Resolution (A)**	**Accuracy**
0.00 ÷ 19.99	0.01	Consider accuracy of line resistance measurement
20.0 ÷ 99.9	0.1	
100 ÷ 999	1	
1.00k ÷ 9.99k	10	
10.0 ÷ 100.0	100	

Test current (at 230 V)..... 3.4 A, 50Hz Sine wave (10 ms ≤ t_{LOAD} ≤ 15 ms)
Nominal voltage range..... 93V÷134V; 185V÷266V; 321V÷485V (45Hz ÷ 65Hz)

Voltage drop:

Measuring range (%)	**Resolution (%)**	**Accuracy**
0.0 ÷ 9.9	0.1	Consider accuracy of the line measurement (only calculated value)

7.6 Phase rotation

Measuring according to EN61557-7

Nominal mains voltage range..... 50 V_{AC} ÷ 550 V_{AC}
Nominal frequency range ..... 45 Hz ÷ 400 Hz
Result displayed ..... Right:1-2-3 ; Left: 3-2-1

7.7 Voltage and frequency

Measuring range (V)	**Resolution (V)**	**Accuracy**
0 ÷ 550	1	±(2 % of reading + 2 digits)

Frequency range ..... 0 Hz, 45 Hz ÷ 400 Hz

Measuring range (Hz)	**Resolution (Hz)**	**Accuracy**
10 ÷ 499	0.1	± 0.2% + 1 digit

Nominal voltage range..... 10V ÷ 550 V

7.8 Earth Resistance

Measuring range according to EN61557-5 is 100Ohm ÷ 1999 Ω.

Re – Earth resistance, 3-wire, 4-wire

Measuring range (Ω)	**Resolution (Ω)**		**Accuracy**
1.0 ÷ 9999	(1.00 ... 19.99) (20.0 ... 199.9) (200.0 ... 9999)	0.01 0.1 1	±(5 % of reading + 5 digits)

Max. auxiliary earth electrode resistance Rh.....100×RE or 50 kΩ (whichever is lower)
Max. probe resistance Rs .....100×RE or 50 kΩ (whichever is lower)
Rh and Rs values are indicative.

Additional probe resistance error at Rhmax or Rsmax…±(10 % of reading + 10 digits)
Additional error at 3 V voltage noise (50 Hz).....±(5 % of reading + 10 digits)

Open circuit voltage.....< 30 VAC
Short circuit current .....< 30 mA
Test voltage frequency .....126.9 Hz
Test voltage shape .....sine wave

Automatic measurement of auxiliary electrode resistance and probe resistance.

Ro - Specific earth resistance

Measuring range	**Resolution (Ωm)**	**Accuracy**
6.0 Ωm … 99.9 Ωm	0.1 Ωm	± (5 % of reading + 5 digits)
100 Ωm ... 999 Ωm	1 Ωm	± (5 % of reading + 5 digits)
1.00 kΩm ... 9.99 kΩm	0.01 kΩm	±(10% of read.)for Re 2kΩ…19.99kΩ
10.0 kΩm ... 99.9 kΩm	0.1 kΩm	±(10% of read.)for Re 2kΩ…19.99kΩ
100 kΩm ... 9999 kΩm	1 kΩm	±(20% of read.) for Re > 20 kΩ

Principle: $\rho = 2 \cdot \pi \cdot d \cdot Re$, where Re is a measured resistance in 4-wire method and d is distance between the probes.

Rh and Rs values are indicative.

7.9 General data

Power supply voltage ..... 9 V_{DC} (6×1.5 V battery cells, size AA)
Power supply adapter..... 12 V DC / 1000 mA
Battery charging current ..... < 600 mA (internally regulated)
Voltage of charged batteries ..... 9 V_{DC} (6×1.5 V, at fully charged state)
Charging duration time ..... typical 6h
Operation ..... typical 15 h

Overvoltage category ..... CAT III / 600 V; CAT IV / 300 V

Protection classification ..... double insulation
Pollution degree 2
Protection degree ..... IP 42

Display ..... 480X320 TFT LCD

COM-Port……USB

Dimensions (w × h × d)..... 25 cm × 10.7 cm × 13.5 cm
Weight (without battery)..... 1.30 kg

Reference conditions
Reference temperature range ..... 10 ^{O}C ÷ 30 ^{O}C
Reference humidity range ..... 40 %RH ÷ 70 %RH

Operating conditions
Working temperature range ..... 0 ^{O}C ÷ 40 ^{O}C
Maximum relative humidity..... 95 %RH (0 ^{O}C ÷ 40 ^{O}C), non-condensing

Storage conditions
Temperature range .... -10 ^{O}C ÷ +70 ^{O}C
Maximum relative humidity..... 90 %RH (-10 ^{O}C ÷ +40 ^{O}C)
80 %RH (40 ^{O}C ÷ 60 ^{O}C)

The error in operating conditions could be at most the error for reference conditions (specified in the manual for each function) + 1 % of measured value + 1 digit unless otherwise specified.